

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009871.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 18:27
Operator : AJ\MA
Sample : N1400-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/07/2022
Supervised By :Ankita Jodhani 02/07/2022

Integration File: Sample.e
Quant Time: Feb 04 22:03:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.431	1816350	13.899 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009871.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 18:27
Operator : AJ\MA
Sample : N1400-01
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/07/2022
Supervised By :Ankita Jodhani 02/07/2022

Integration File: Sample.e
Quant Time: Feb 04 22:03:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

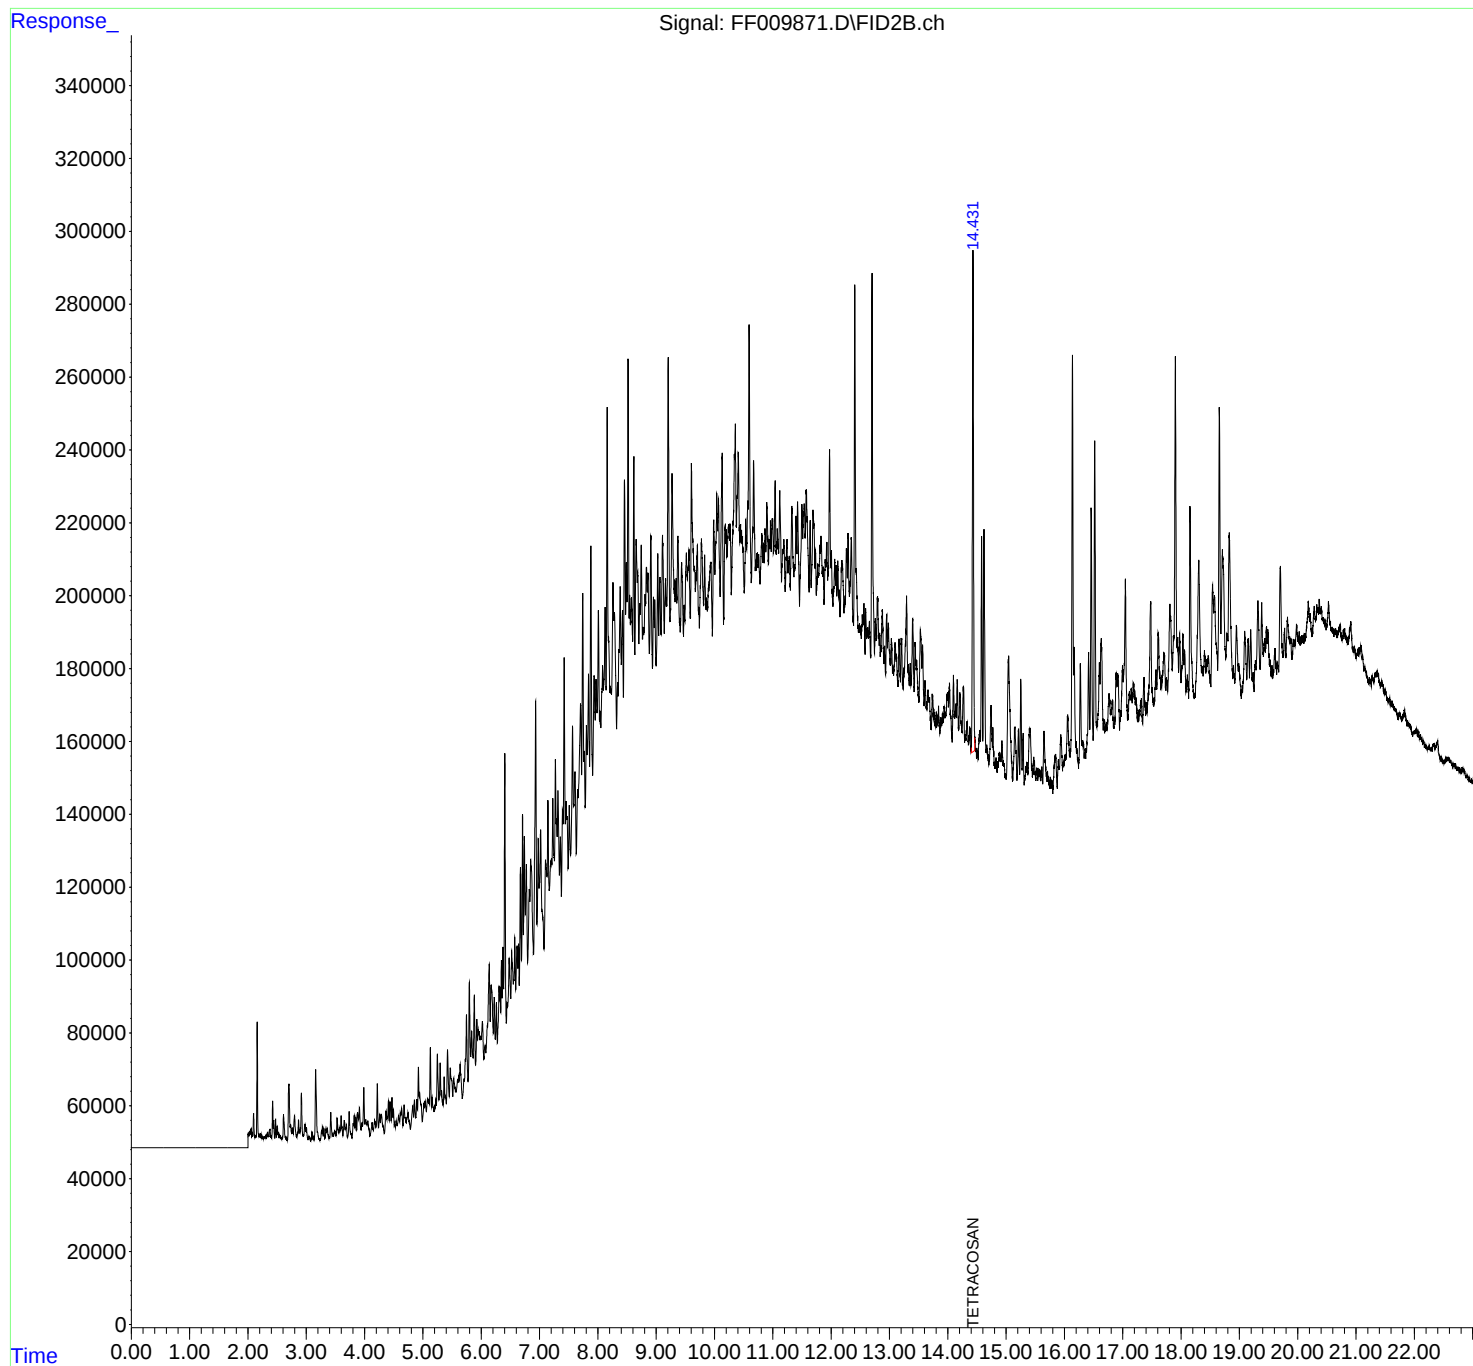

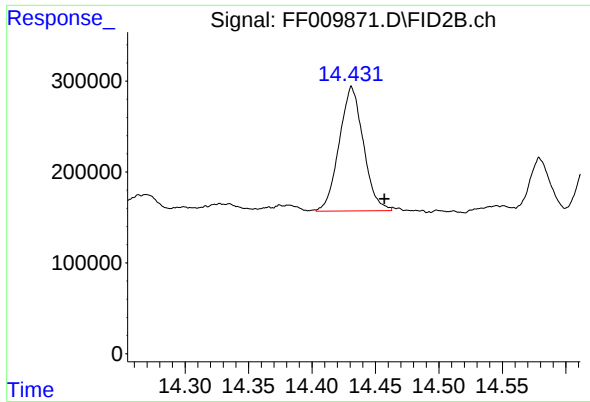

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.431 min
Delta R.T.: -0.026 min
Response: 1816350
Conc: 13.90 ug/ml

Instrument :

FID_F

ClientSampleId :

KTS1-WC-S-MH-01-02-0-15

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/07/2022
Supervised By :Ankita Jodhani 02/07/2022