

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020422\  
 Data File : FF009886.D  
 Signal(s) : FID2B.ch  
 Acq On : 05 Feb 2022 02:17  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 I.BLK

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 02/07/2022  
 Supervised By :Ankita Jodhani 02/07/2022

Integration File: Sample.e  
 Quant Time: Feb 05 03:52:46 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
 Quant Title :  
 QLast Update : Tue Jan 18 02:53:40 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.422 | 2307108  | 17.655 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020422\  
Data File : FF009886.D  
Signal(s) : FID2B.ch  
Acq On : 05 Feb 2022 02:17  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
I.BLK


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/07/2022  
Supervised By :Ankita Jodhani 02/07/2022

Integration File: Sample.e  
Quant Time: Feb 05 03:52:46 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
Quant Title :  
QLast Update : Tue Jan 18 02:53:40 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

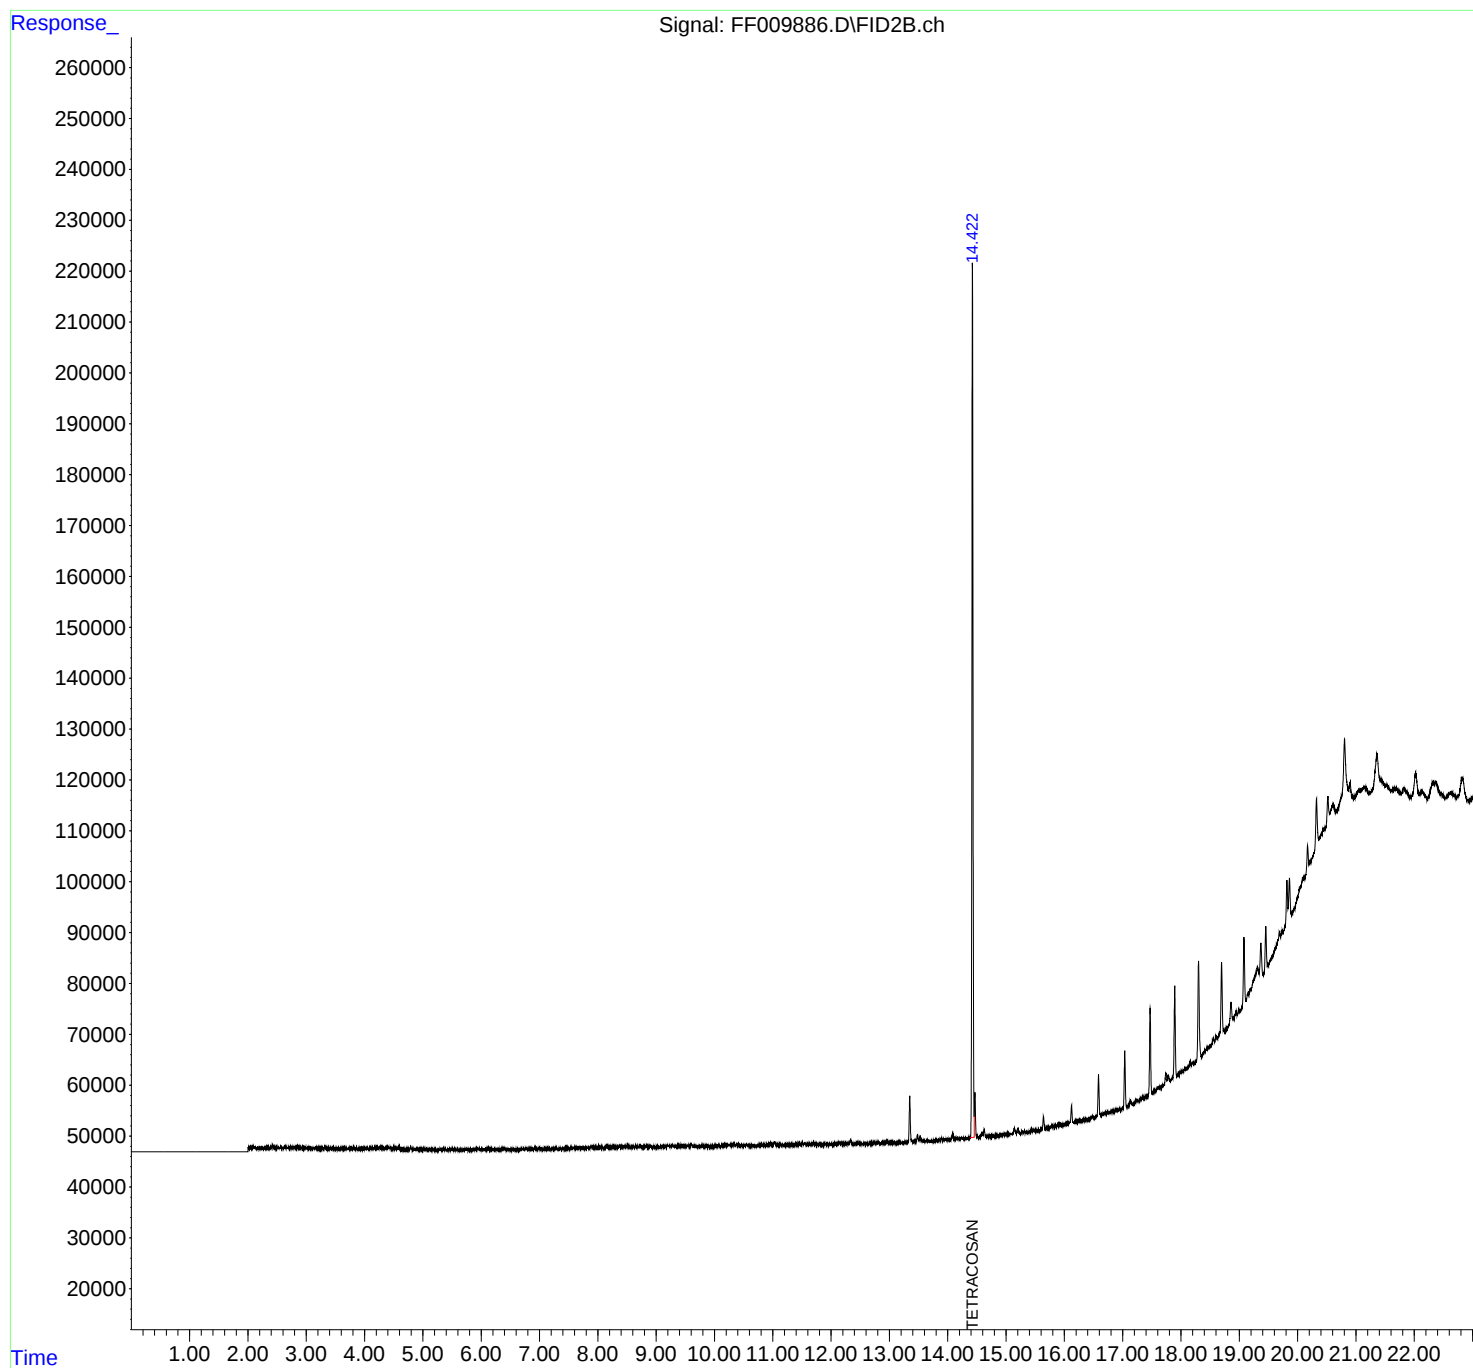

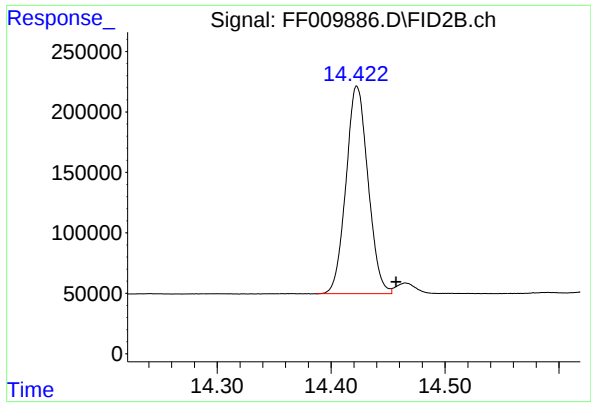

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.422 min  
Delta R.T.: -0.035 min  
Response: 2307108  
Conc: 17.65 ug/ml

Instrument :

FID\_F

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/07/2022

Supervised By :Ankita Jodhani 02/07/2022