

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020619\
Data File : FF003394.D
Signal(s) : FID2B.ch
Acq On : 06 Feb 2019 12:32
Operator : AJ\SJ
Sample : K1341-01 50X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 07 00:05:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.344	196652	1.469 ug/ml
3) N-DODECANE	6.362	597881	4.434 ug/ml
4) N-TETRADECANE	8.155	472170	3.488 ug/ml
5) N-HEXADECANE	9.755	259499	1.904 ug/ml
6) N-OCTADECANE	11.199	133360	0.969 ug/ml
7) N-EICOSANE	12.512	84662	0.616 ug/ml
13) N-TRIACONTANE	17.693	66766	0.473 ug/ml
14) N-DOTRIACONTANE	18.530	143516	1.040 ug/ml
15) N-TETRATRIACONTANE	19.317	50170	0.396 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020619\
Data File : FF003394.D
Signal(s) : FID2B.ch
Acq On : 06 Feb 2019 12:32
Operator : AJ\SJ
Sample : K1341-01 50X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 07 00:05:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

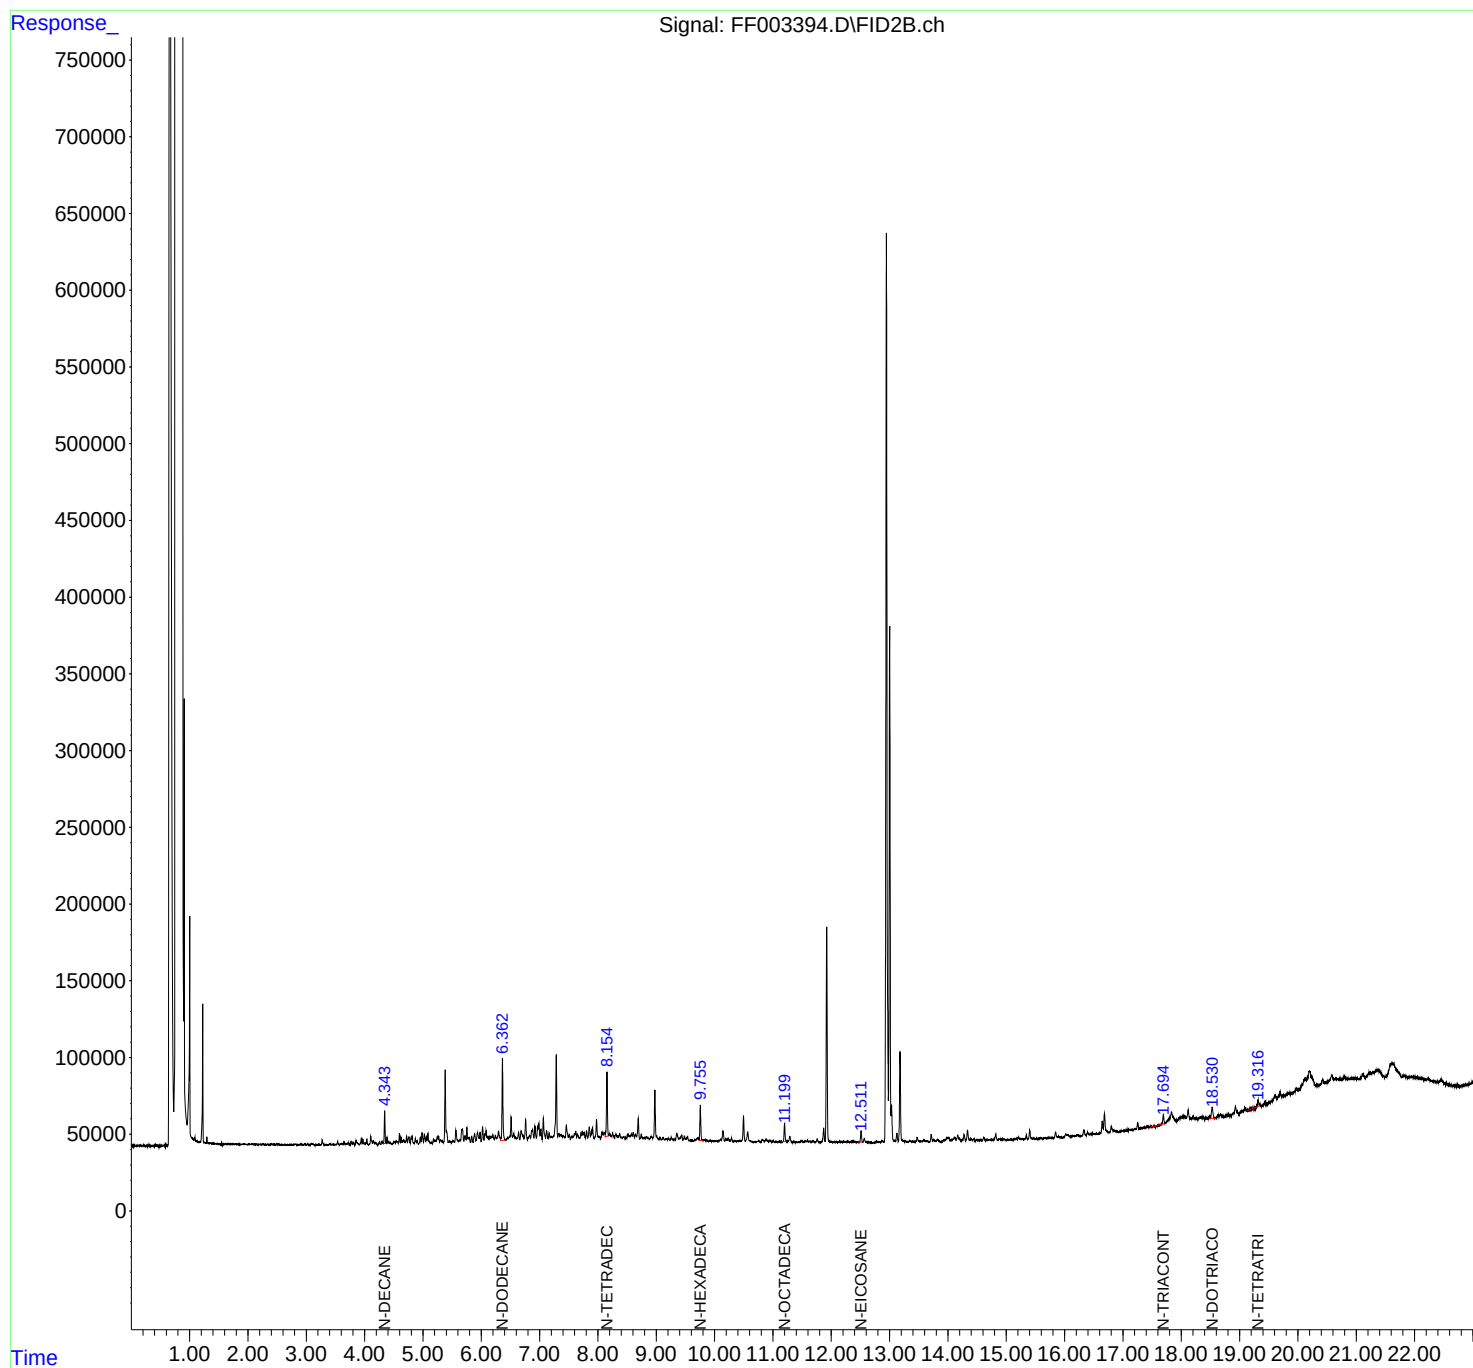

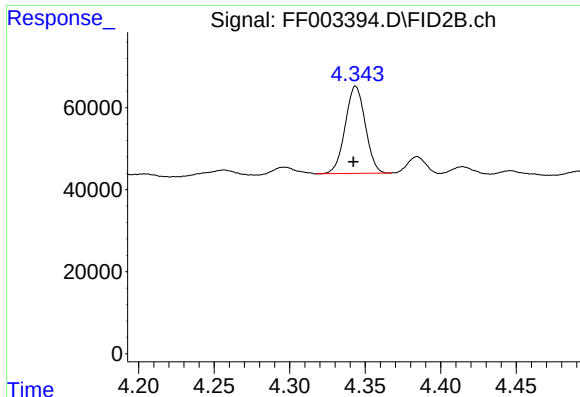


#2 N-DECANE

R.T.: 4.344 min
Delta R.T.: 0.002 min
Response: 196652
Conc: 1.47 ug/ml

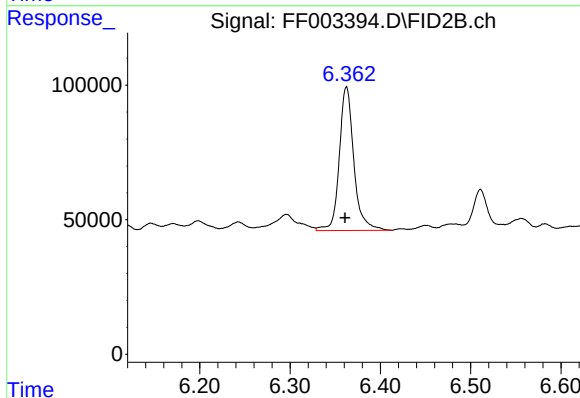


#3 N-DODECANE

R.T.: 6.362 min
Delta R.T.: 0.001 min
Response: 597881
Conc: 4.43 ug/ml

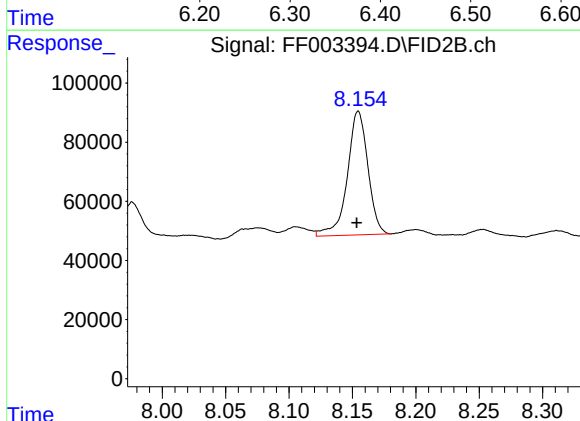


#4 N-TETRADECANE

R.T.: 8.155 min
Delta R.T.: 0.001 min
Response: 472170
Conc: 3.49 ug/ml

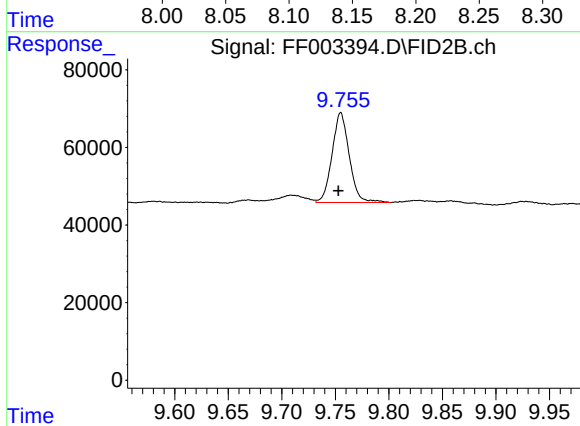


#5 N-HEXADECANE

R.T.: 9.755 min
Delta R.T.: 0.002 min
Response: 259499
Conc: 1.90 ug/ml

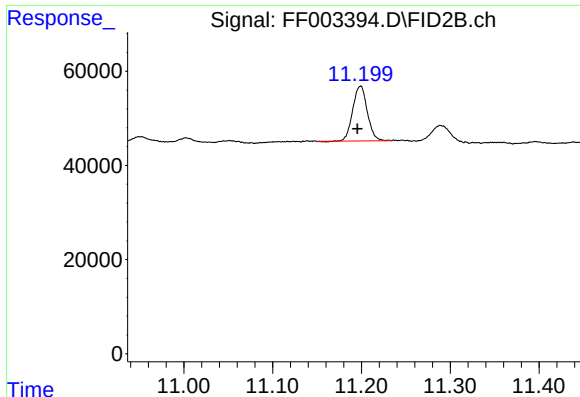


#6 N-OCTADECANE

R.T.: 11.199 min
Delta R.T.: 0.003 min
Response: 133360
Conc: 0.97 ug/ml

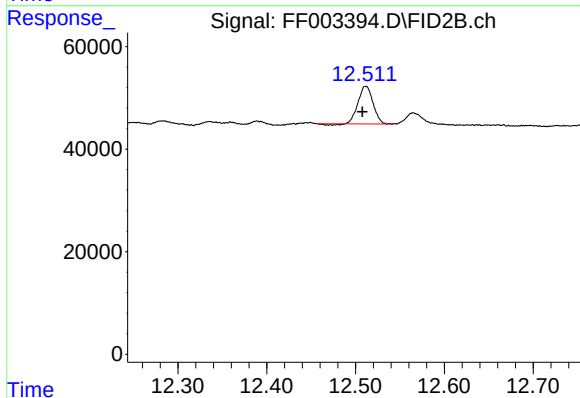


#7 N-EICOSANE

R.T.: 12.512 min
Delta R.T.: 0.004 min
Response: 84662
Conc: 0.62 ug/ml

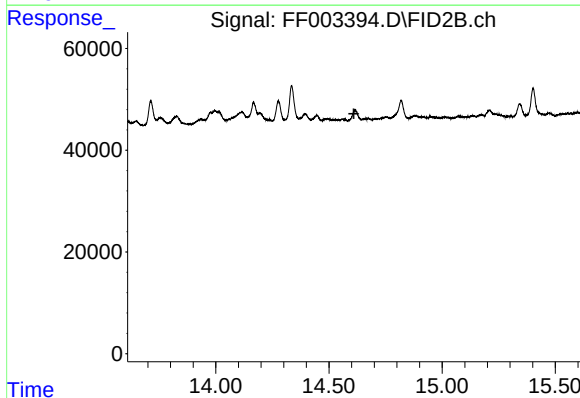


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.610 min
Response: 0
Conc: N.D.

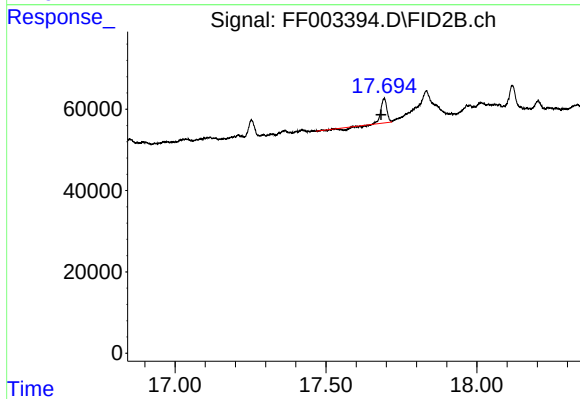


#13 N-TRIACONTANE

R.T.: 17.693 min
Delta R.T.: 0.010 min
Response: 66766
Conc: 0.47 ug/ml

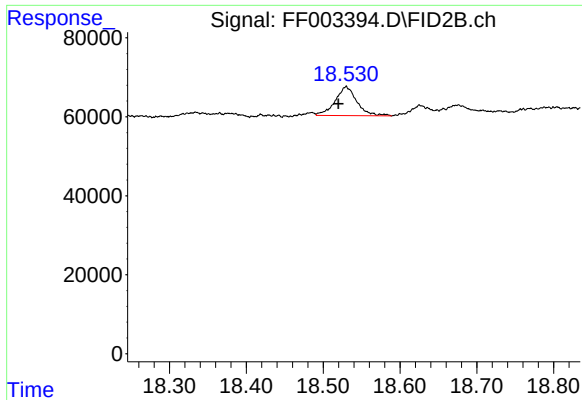

#14 N-DOTRIACONTANE

R.T.: 18.530 min
Delta R.T.: 0.010 min
Response: 143516
Conc: 1.04 ug/ml

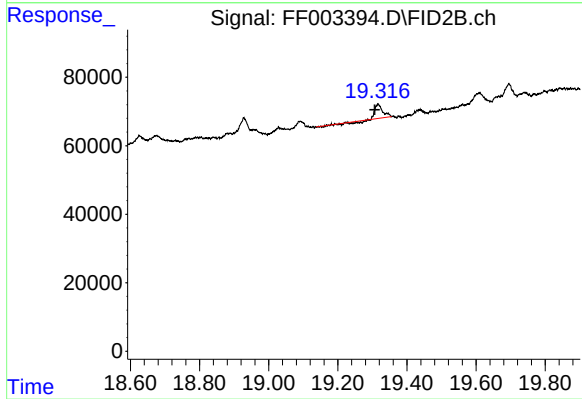

#15 N-TETRATRIACONTANE

R.T.: 19.317 min
Delta R.T.: 0.009 min
Response: 50170
Conc: 0.40 ug/ml