

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020619\
 Data File : FF003396.D
 Signal(s) : FID2B.ch
 Acq On : 06 Feb 2019 13:31
 Operator : AJ\SJ
 Sample : K1350-03 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 07 00:05:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	758961	6.287 ug/ml
Target Compounds			
3) N-DODECANE	6.367	92219	0.684 ug/ml
4) N-TETRADECANE	8.160	108525	0.802 ug/ml
5) N-HEXADECANE	9.761	106898	0.784 ug/ml
7) N-EICOSANE	12.571f	207946	1.512 ug/ml
10) N-TETRACOSANE	14.797	45494	0.335 ug/ml
11) N-HEXACOSANE	15.852	98934	0.729 ug/ml
12) N-OCTACOSANE	16.807	235092	1.717 ug/ml
13) N-TRIACONTANE	17.697	254392	1.802 ug/ml
14) N-DOTRIACONTANE	18.536	254772	1.846 ug/ml
15) N-TETRATRIACONTANE	19.322	9877	0.078 ug/ml
16) N-HEXATRIACONTANE	20.074	61014	0.522 ug/ml
18) N-TETRACONTANE	21.732	490608	4.531 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020619\
Data File : FF003396.D
Signal(s) : FID2B.ch
Acq On : 06 Feb 2019 13:31
Operator : AJ\SJ
Sample : K1350-03 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 07 00:05:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

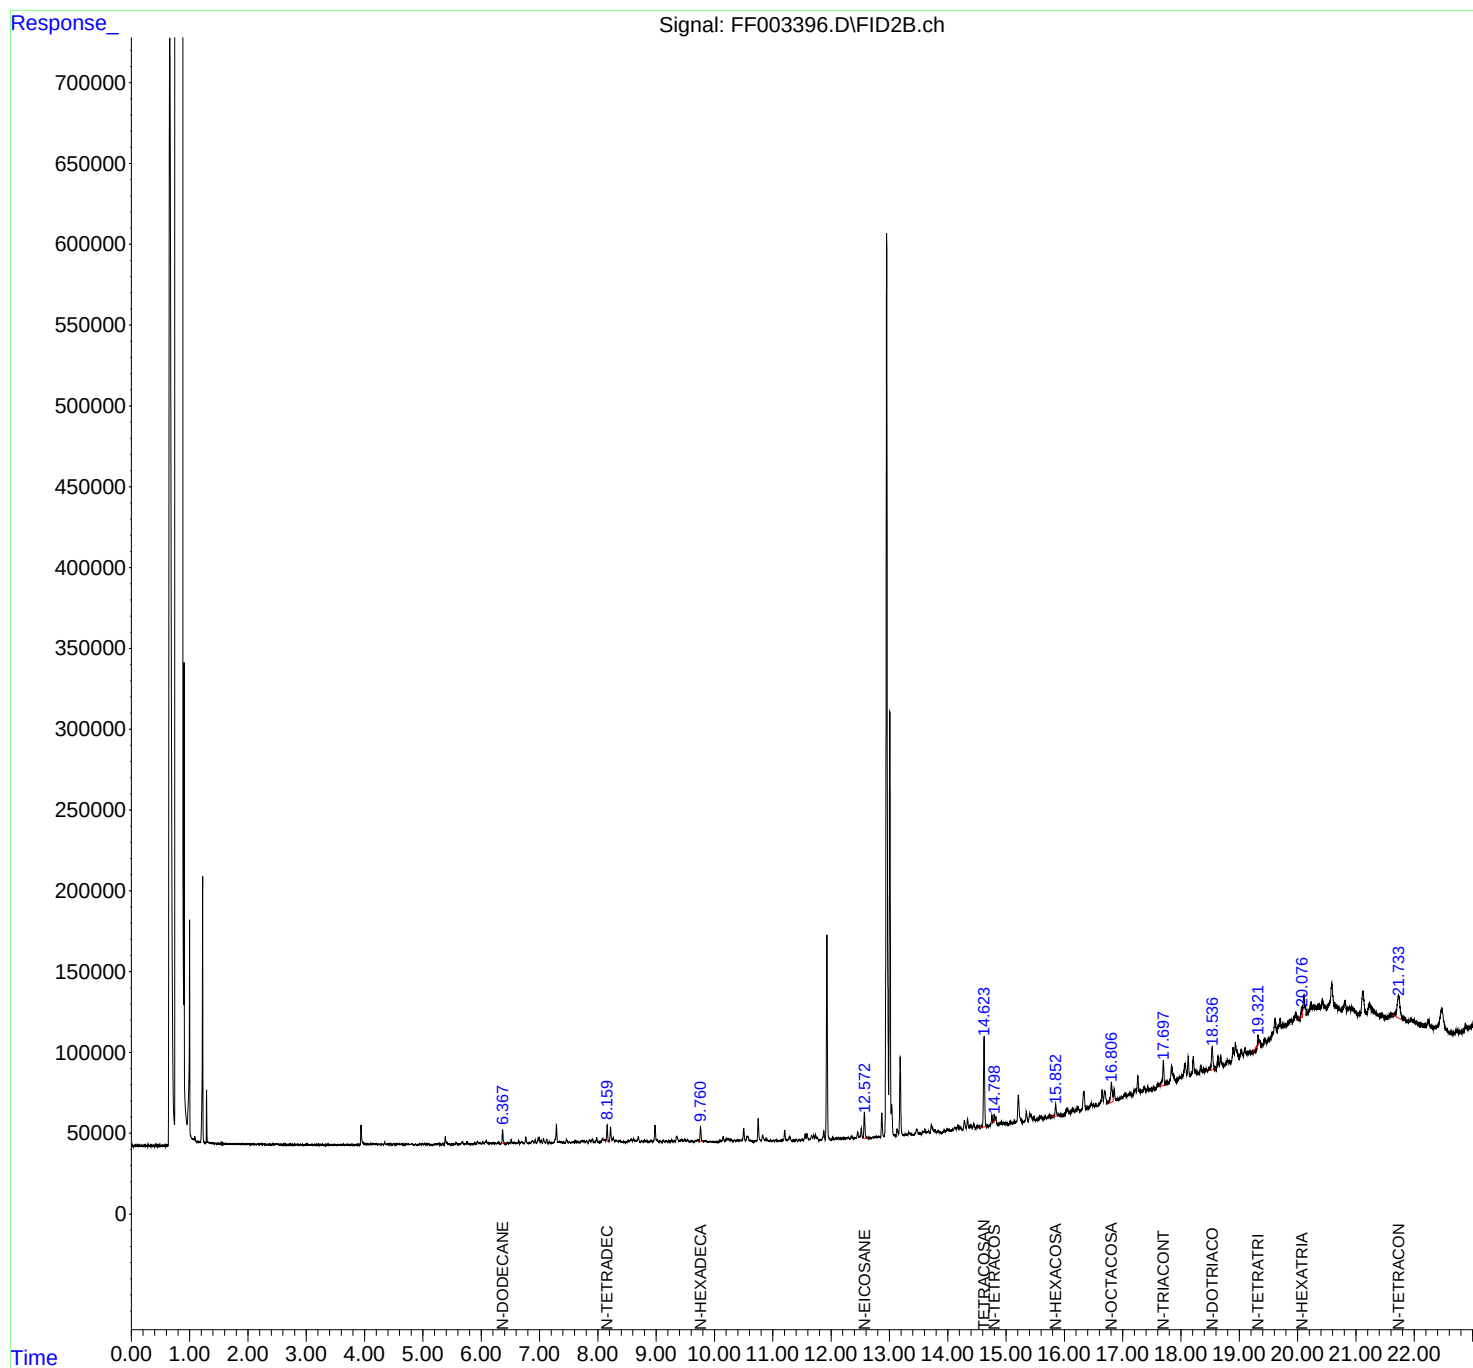

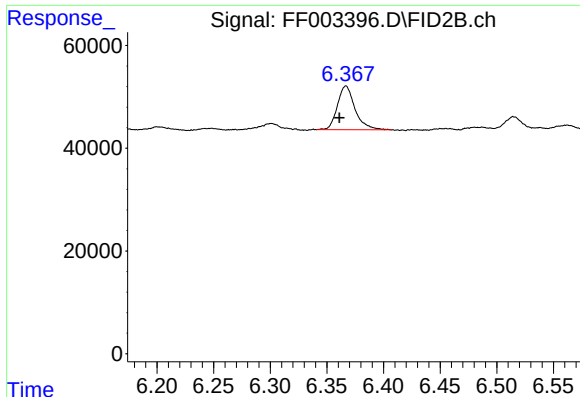


#3 N-DODECANE

R.T.: 6.367 min
Delta R.T.: 0.006 min
Response: 92219
Conc: 0.68 ug/ml

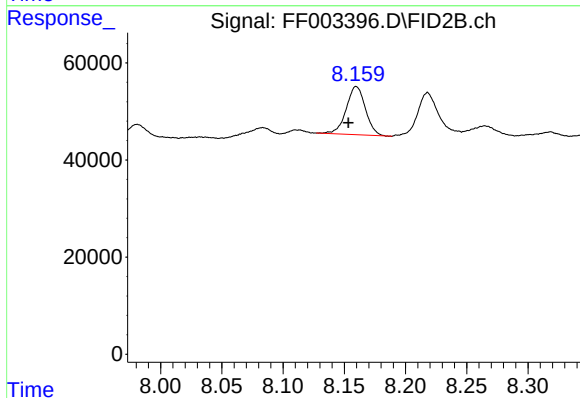


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: 0.006 min
Response: 108525
Conc: 0.80 ug/ml

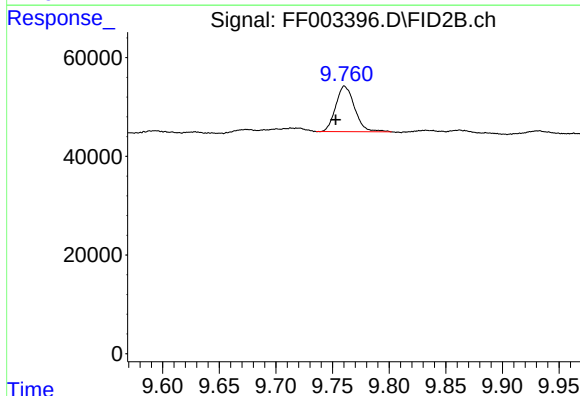


#5 N-HEXADECANE

R.T.: 9.761 min
Delta R.T.: 0.008 min
Response: 106898
Conc: 0.78 ug/ml

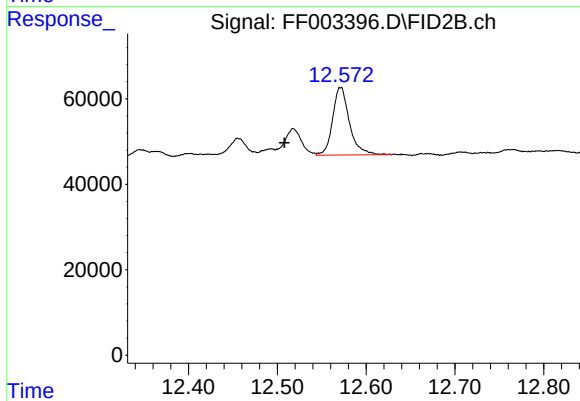


#7 N-EICOSANE

R.T.: 12.571 min
Delta R.T.: 0.064 min
Response: 207946
Conc: 1.51 ug/ml

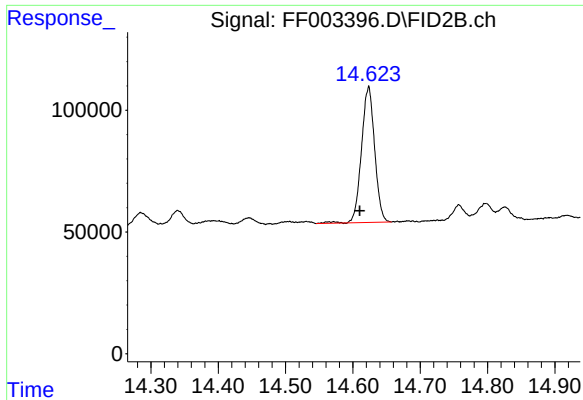


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.623 min
Delta R.T.: 0.013 min
Response: 758961
Conc: 6.29 ug/ml

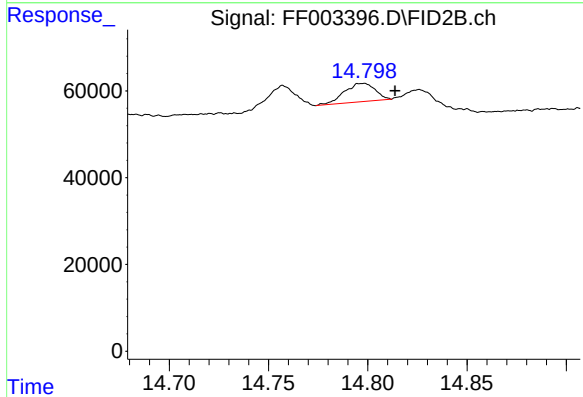


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: -0.016 min
Response: 45494
Conc: 0.33 ug/ml

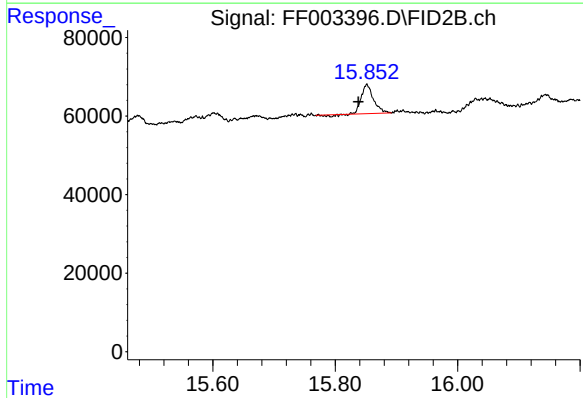


#11 N-HEXACOSANE

R.T.: 15.852 min
Delta R.T.: 0.013 min
Response: 98934
Conc: 0.73 ug/ml

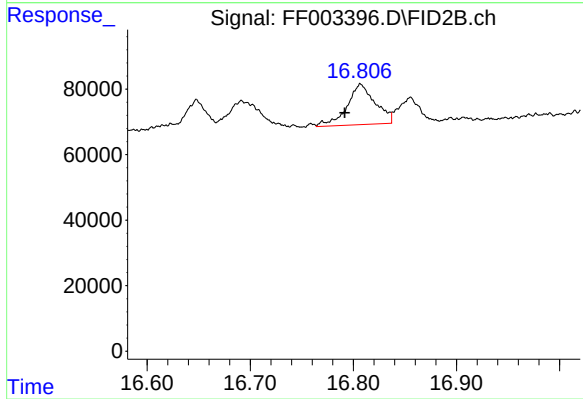


#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: 0.016 min
Response: 235092
Conc: 1.72 ug/ml

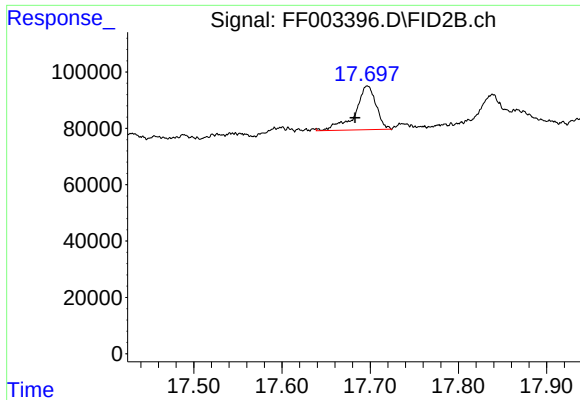


#13 N-TRIACONTANE

R.T.: 17.697 min
Delta R.T.: 0.014 min
Response: 254392
Conc: 1.80 ug/ml

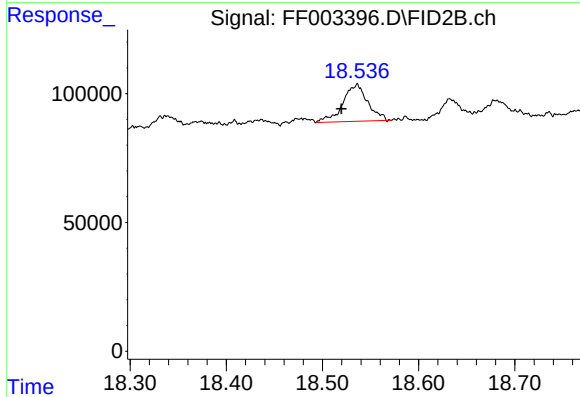


#14 N-DOTRIACONTANE

R.T.: 18.536 min
Delta R.T.: 0.016 min
Response: 254772
Conc: 1.85 ug/ml

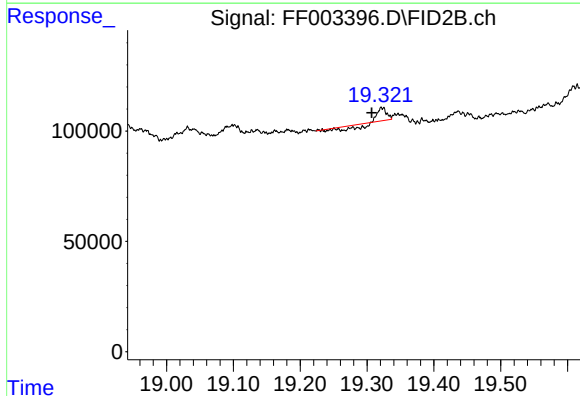


#15 N-TETRATRIACONTANE

R.T.: 19.322 min
Delta R.T.: 0.015 min
Response: 9877
Conc: 0.08 ug/ml

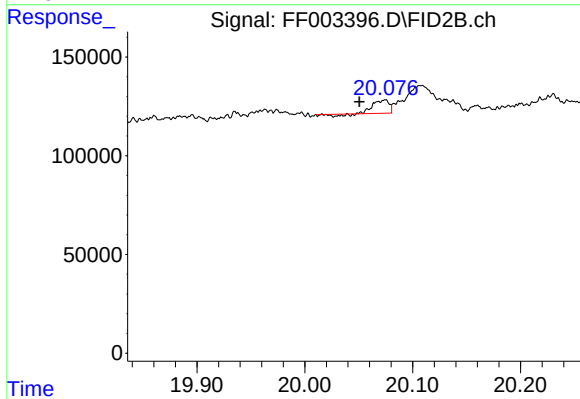

#16 N-HEXATRIACONTANE

R.T.: 20.074 min
Delta R.T.: 0.024 min
Response: 61014
Conc: 0.52 ug/ml

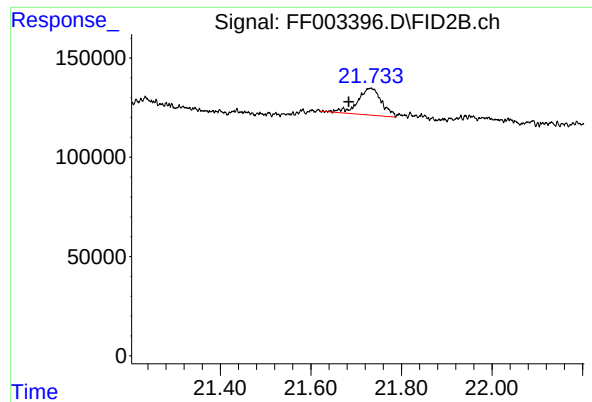

#18 N-TETRACONTANE

R.T.: 21.732 min
Delta R.T.: 0.049 min
Response: 490608
Conc: 4.53 ug/ml