

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020619\  
Data File : FF003407.D  
Signal(s) : FID2B.ch  
Acq On : 06 Feb 2019 19:37  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Feb 07 00:08:37 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF020119.M  
Quant Title :  
QLast Update : Fri Feb 01 22:57:49 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.    | Response | Conc Units  |
|-----------------------------|---------|----------|-------------|
| -----                       |         |          |             |
| System Monitoring Compounds |         |          |             |
| Target Compounds            |         |          |             |
| 14) N-DOTRIACONTANE         | 18.534  | 150342   | 1.089 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.105f | 417374   | 3.570 ug/ml |
| -----                       |         |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020619\  
Data File : FF003407.D  
Signal(s) : FID2B.ch  
Acq On : 06 Feb 2019 19:37  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Feb 07 00:08:37 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF020119.M  
Quant Title :  
QLast Update : Fri Feb 01 22:57:49 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

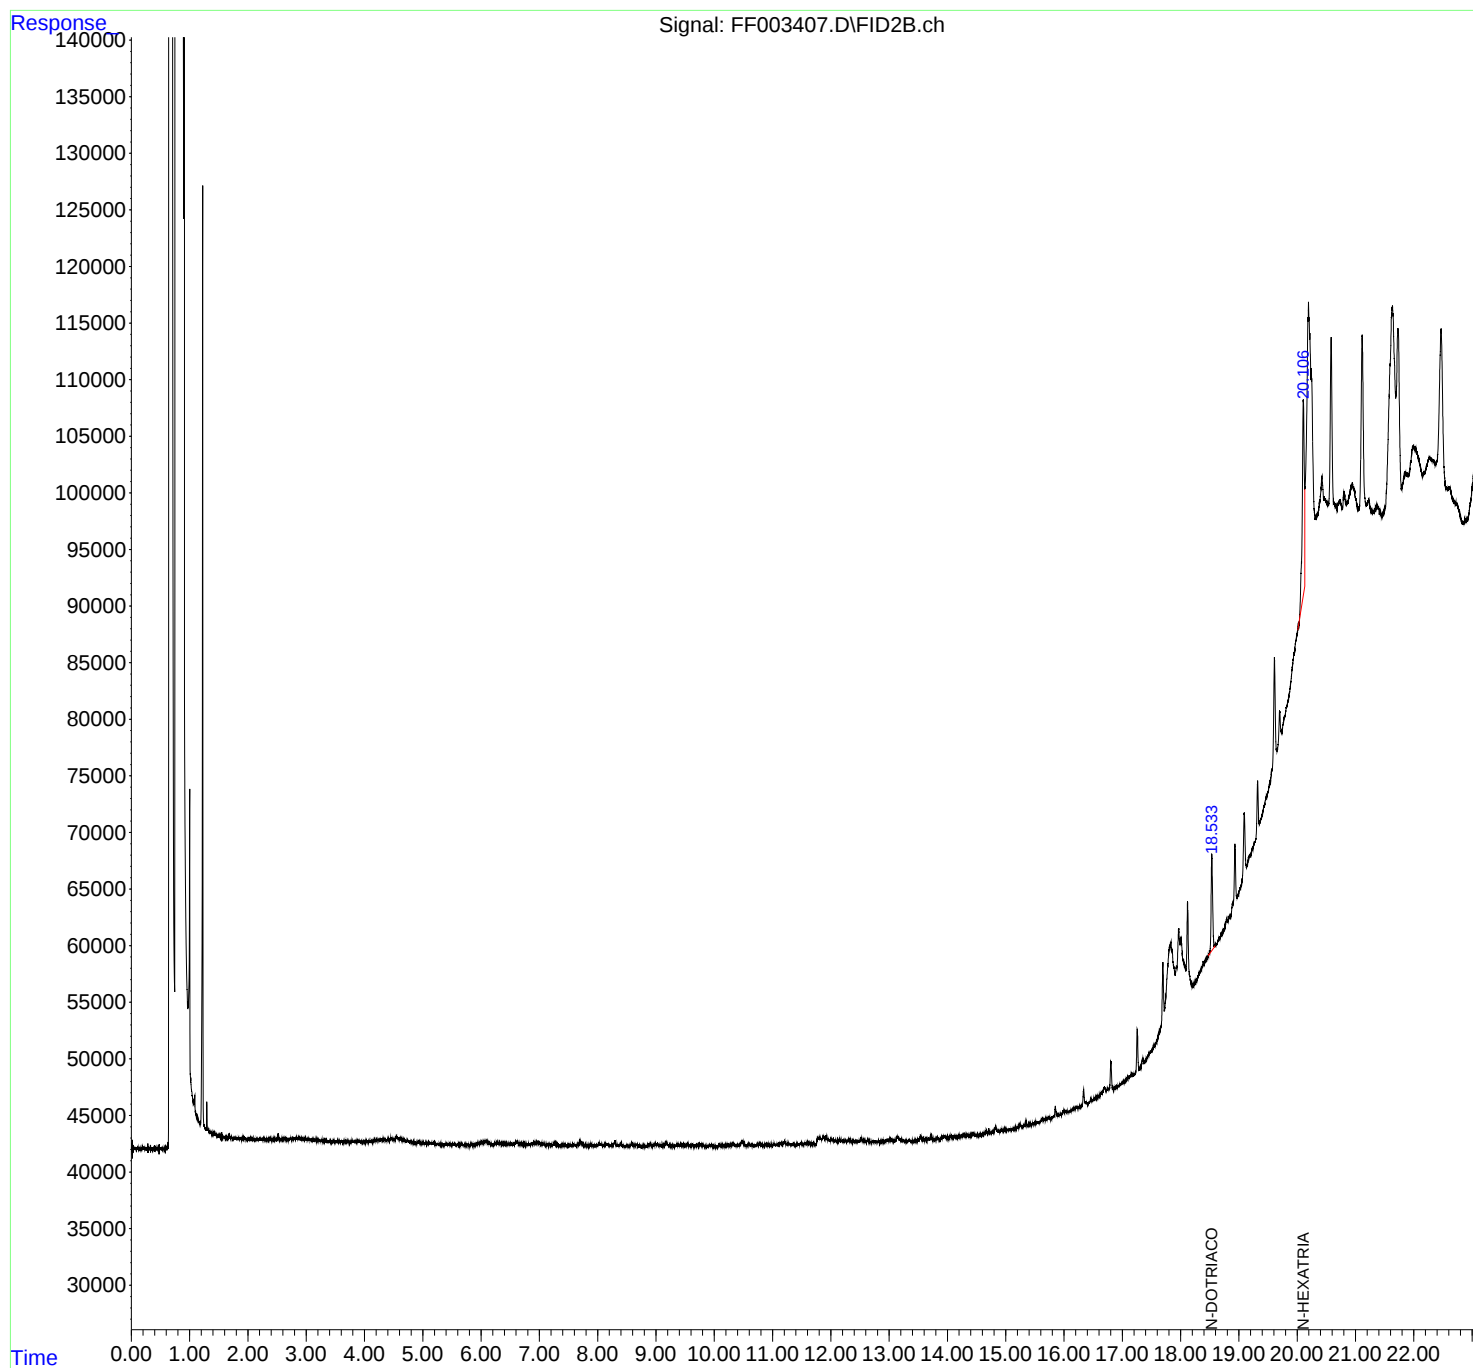

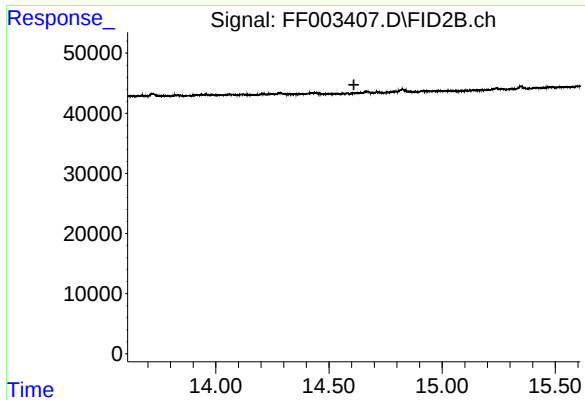


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.610 min  
Response: 0  
Conc: N.D.

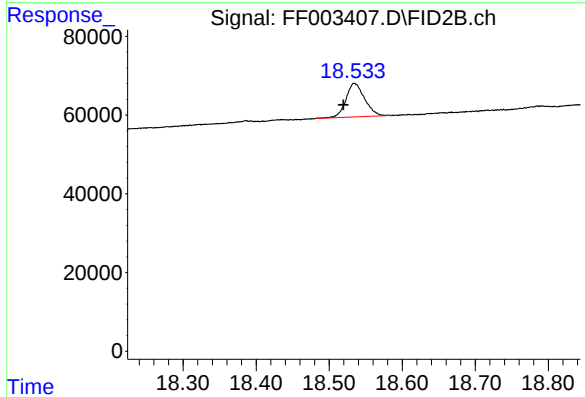

#14 N-DOTRIACONTANE

R.T.: 18.534 min  
Delta R.T.: 0.015 min  
Response: 150342  
Conc: 1.09 ug/ml

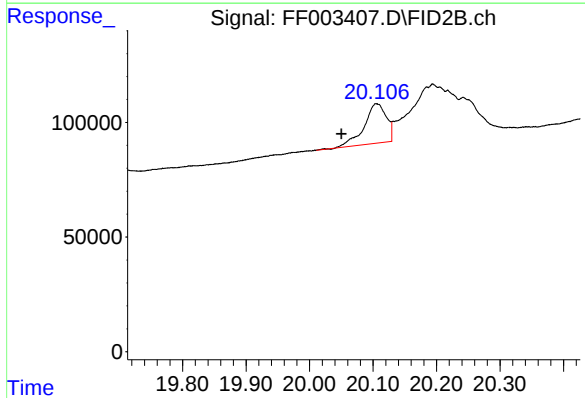

#16 N-HEXATRIACONTANE

R.T.: 20.105 min  
Delta R.T.: 0.055 min  
Response: 417374  
Conc: 3.57 ug/ml