

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF020719\
 Data File : FF003416.D
 Signal(s) : FID2B.ch
 Acq On : 07 Feb 2019 16:55
 Operator : AJ\SJ
 Sample : K1392-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 08 08:04:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.619	2079989	17.229 ug/ml
Target Compounds			
2) N-DECANE	4.384	3734117	27.902 ug/ml
3) N-DODECANE	6.365	399533	2.963 ug/ml
4) N-TETRADECANE	8.220f	209014	1.544 ug/ml
5) N-HEXADECANE	9.786	1947318	14.289 ug/ml
12) N-OCTACOSANE	16.800	101638	0.742 ug/ml
13) N-TRIACONTANE	17.690	126992	0.899 ug/ml
14) N-DOTRIACONTANE	18.527	200990	1.456 ug/ml
16) N-HEXATRIACONTANE	20.099	386157	3.303 ug/ml
18) N-TETRACONTANE	21.728	542820	5.014 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF020719\
Data File : FF003416.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2019 16:55
Operator : AJ\SJ
Sample : K1392-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 08:04:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

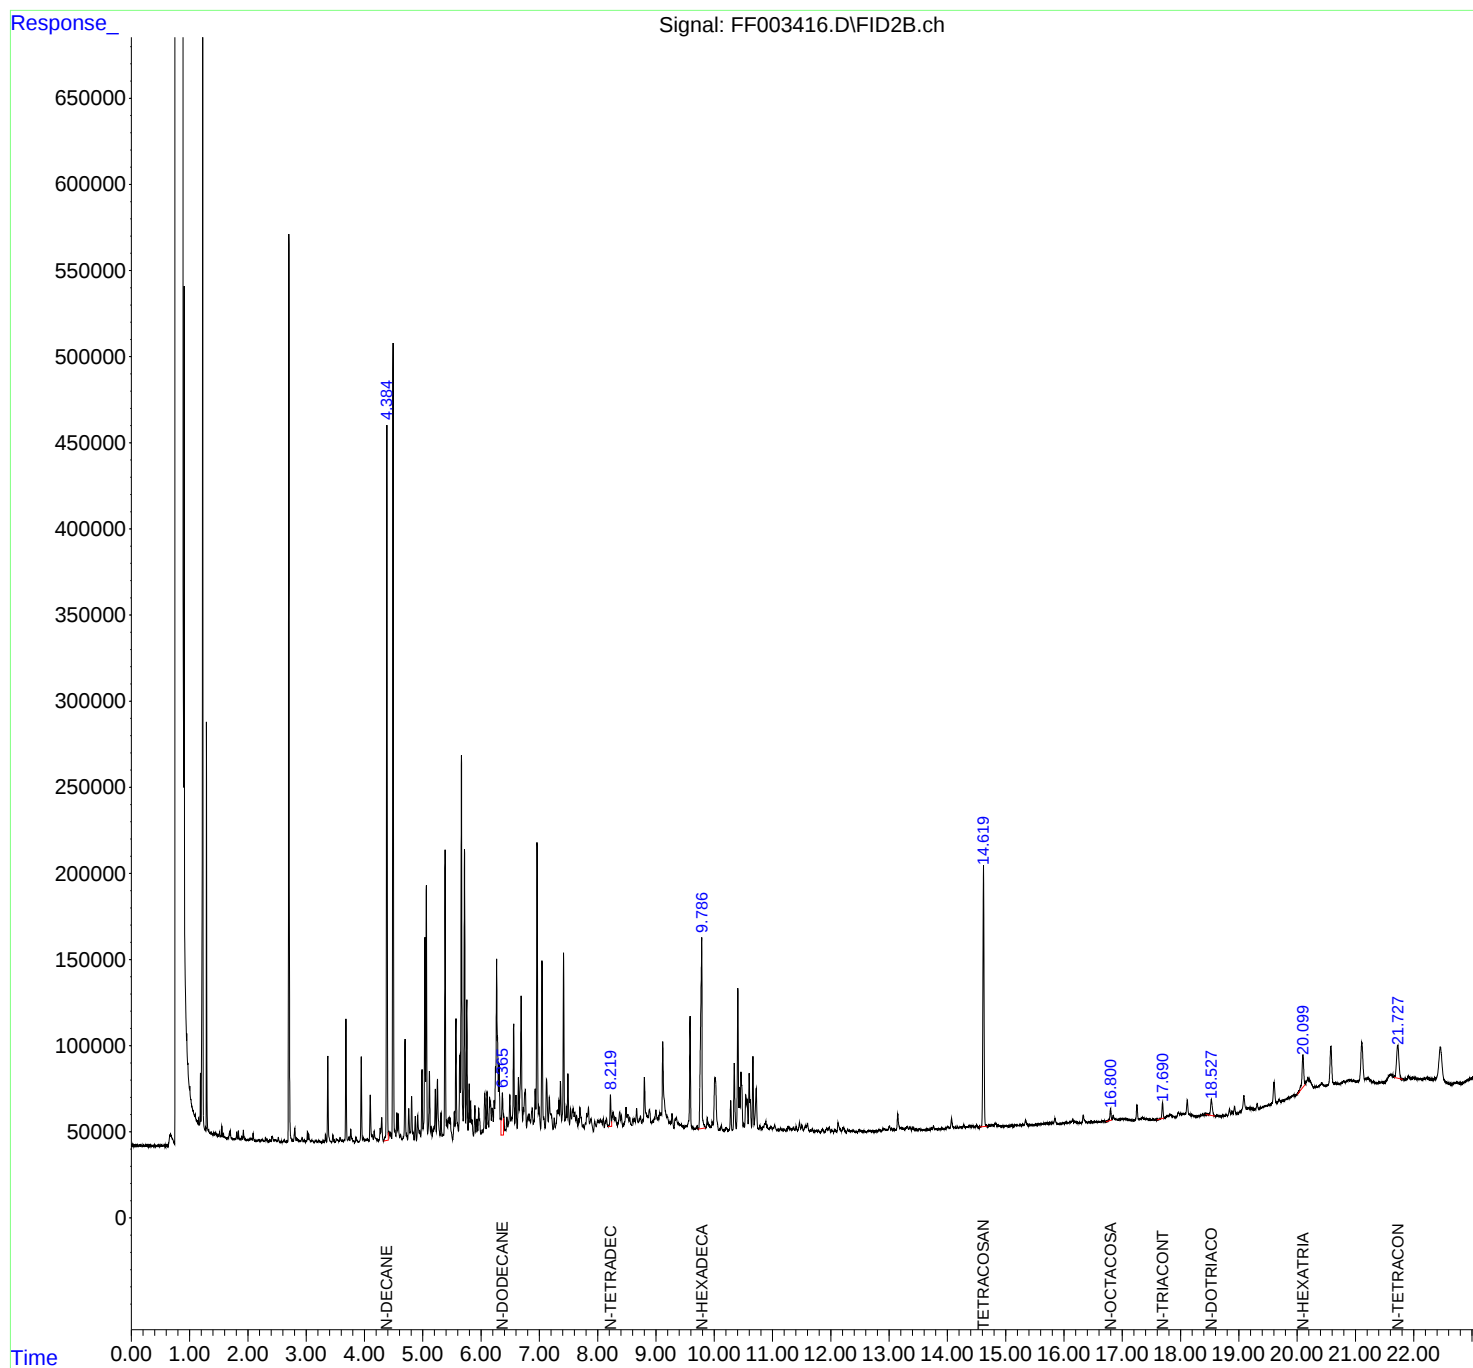

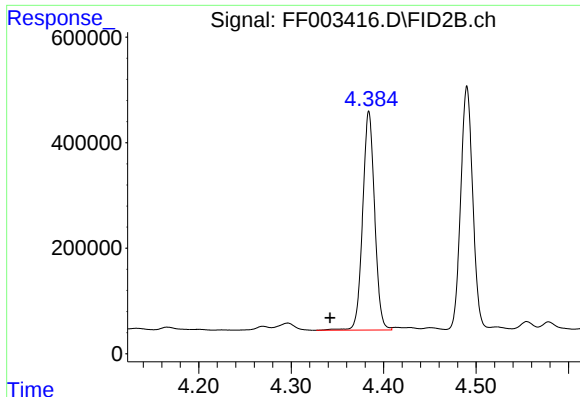


#2 N-DECANE

R.T.: 4.384 min
Delta R.T.: 0.042 min
Response: 3734117
Conc: 27.90 ug/ml

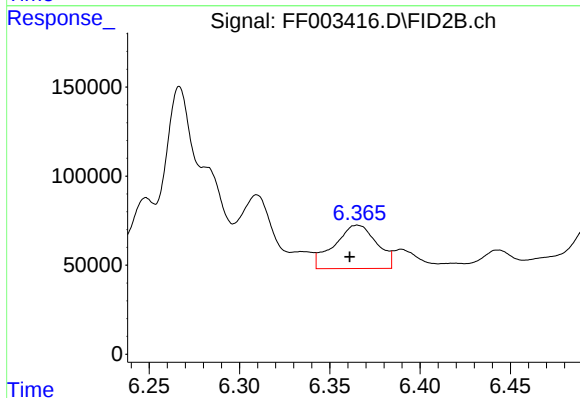


#3 N-DODECANE

R.T.: 6.365 min
Delta R.T.: 0.004 min
Response: 399533
Conc: 2.96 ug/ml

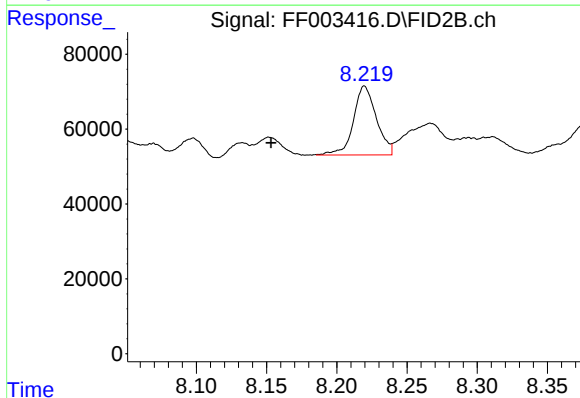


#4 N-TETRADECANE

R.T.: 8.220 min
Delta R.T.: 0.066 min
Response: 209014
Conc: 1.54 ug/ml

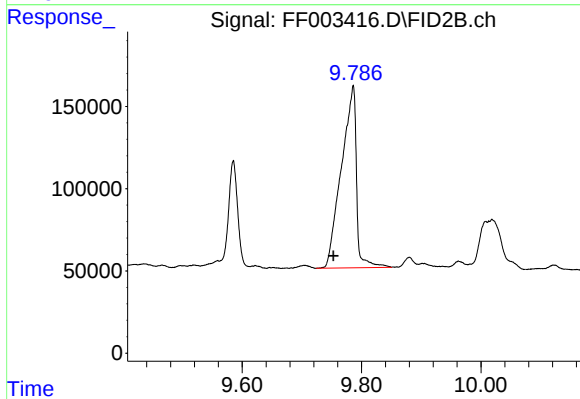


#5 N-HEXADECANE

R.T.: 9.786 min
Delta R.T.: 0.033 min
Response: 1947318
Conc: 14.29 ug/ml

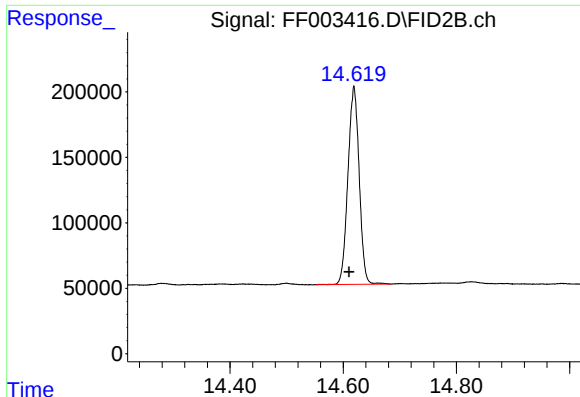


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.619 min
Delta R.T.: 0.009 min
Response: 2079989
Conc: 17.23 ug/ml

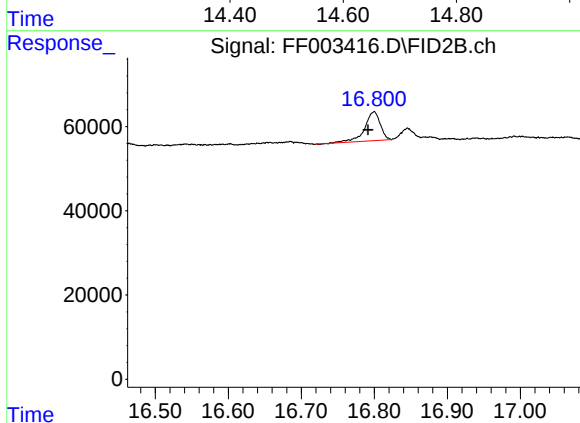


#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.008 min
Response: 101638
Conc: 0.74 ug/ml

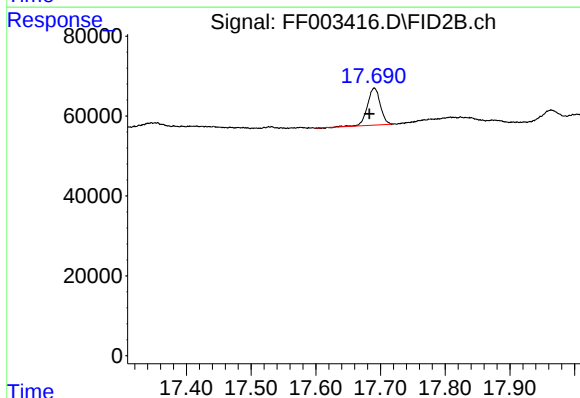


#13 N-TRIACONTANE

R.T.: 17.690 min
Delta R.T.: 0.007 min
Response: 126992
Conc: 0.90 ug/ml

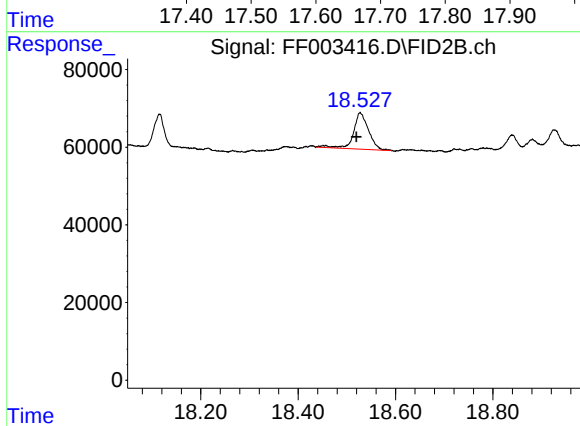


#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: 0.008 min
Response: 200990
Conc: 1.46 ug/ml

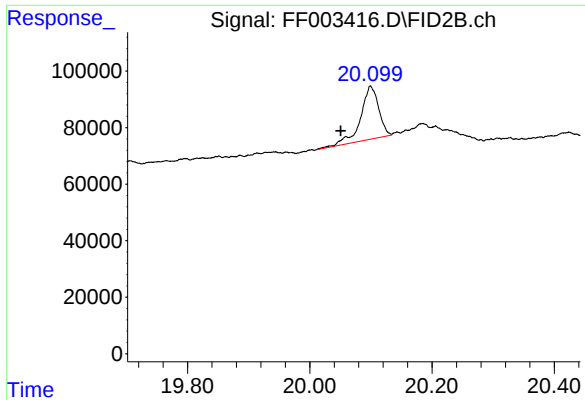

#16 N-HEXATRIACONTANE

R.T.: 20.099 min
Delta R.T.: 0.049 min
Response: 386157
Conc: 3.30 ug/ml

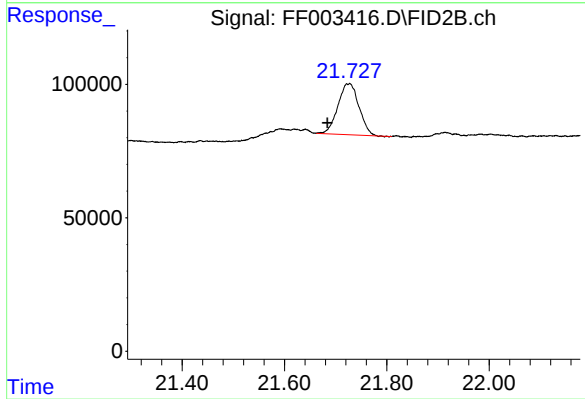

#18 N-TETRACONTANE

R.T.: 21.728 min
Delta R.T.: 0.044 min
Response: 542820
Conc: 5.01 ug/ml