

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009888.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 09:55
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:55:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.308	173983	1.279 ug/ml
15)	N-TETRATRIACONTANE	19.083	307567	2.590 ug/ml
16)	N-HEXATRIACONTANE	19.857	599476	5.814 ug/ml
18)	N-TETRACONTANE	21.358	81313	0.895 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009888.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 09:55
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:55:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

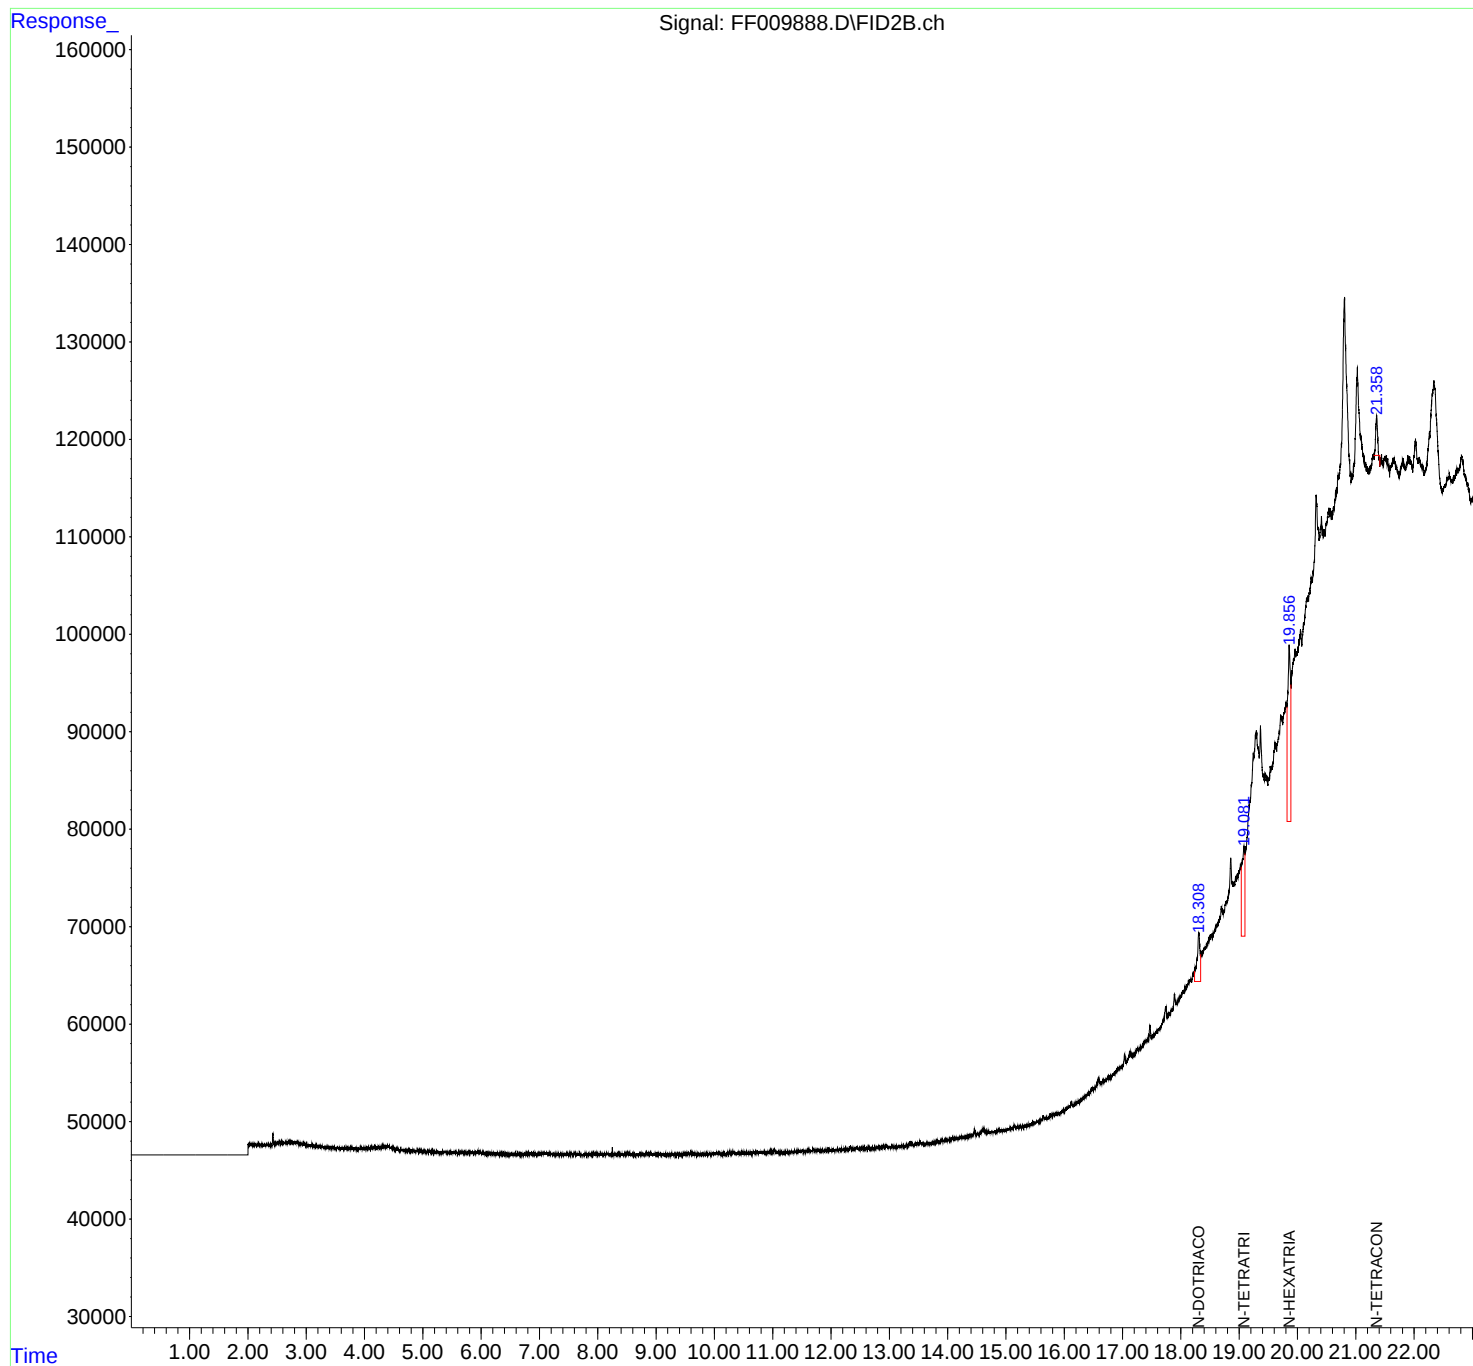


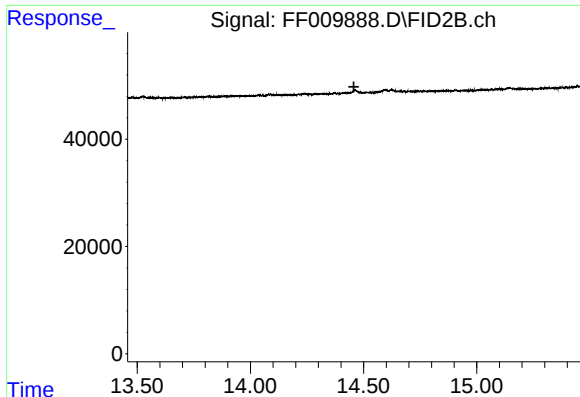

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

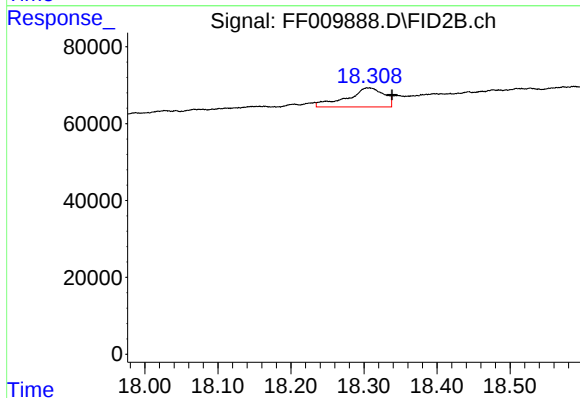


#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: -0.031 min
Response: 173983
Conc: 1.28 ug/ml

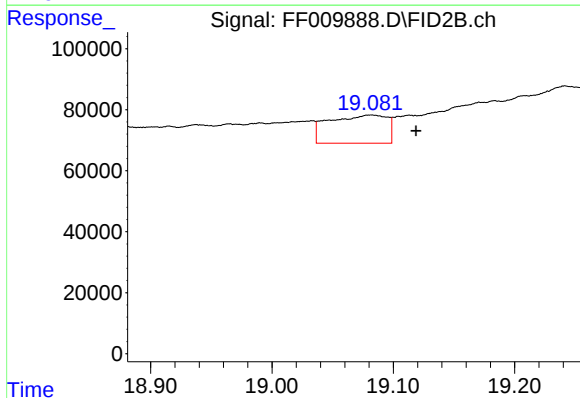


#15 N-TETRATRIACONTANE

R.T.: 19.083 min
Delta R.T.: -0.036 min
Response: 307567
Conc: 2.59 ug/ml

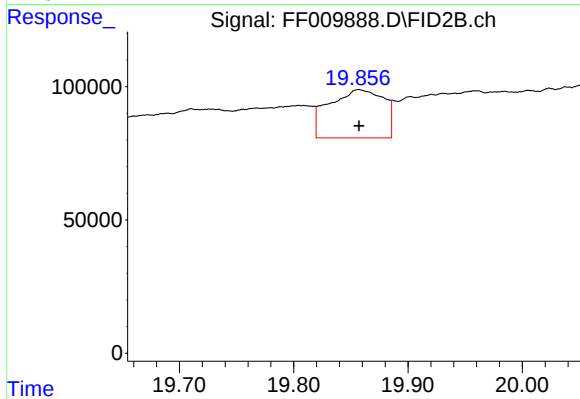

#16 N-HEXATRIACONTANE

R.T.: 19.857 min
Delta R.T.: 0.000 min
Response: 599476
Conc: 5.81 ug/ml

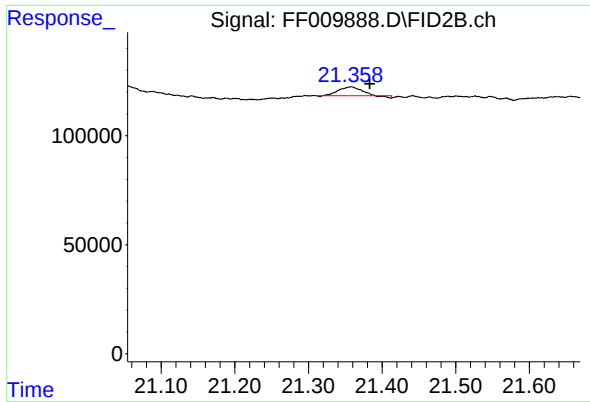

#18 N-TETRACONTANE

R.T.: 21.358 min
Delta R.T.: -0.025 min
Response: 81313
Conc: 0.90 ug/ml

Instrument :

FID_F

ClientSampleId :