

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009891.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 13:13
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:56:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.220	3979273	27.808 ug/ml
12)	N-OCTACOSANE	16.589	3221547	22.192 ug/ml
13)	N-TRIACONTANE	17.469	65760	0.460 ug/ml
14)	N-DOTRIACONTANE	18.299	96672	0.710 ug/ml
15)	N-TETRATRIACONTANE	19.079	189263	1.593 ug/ml
16)	N-HEXATRIACONTANE	19.858	163546	1.586 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009891.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 13:13
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:56:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

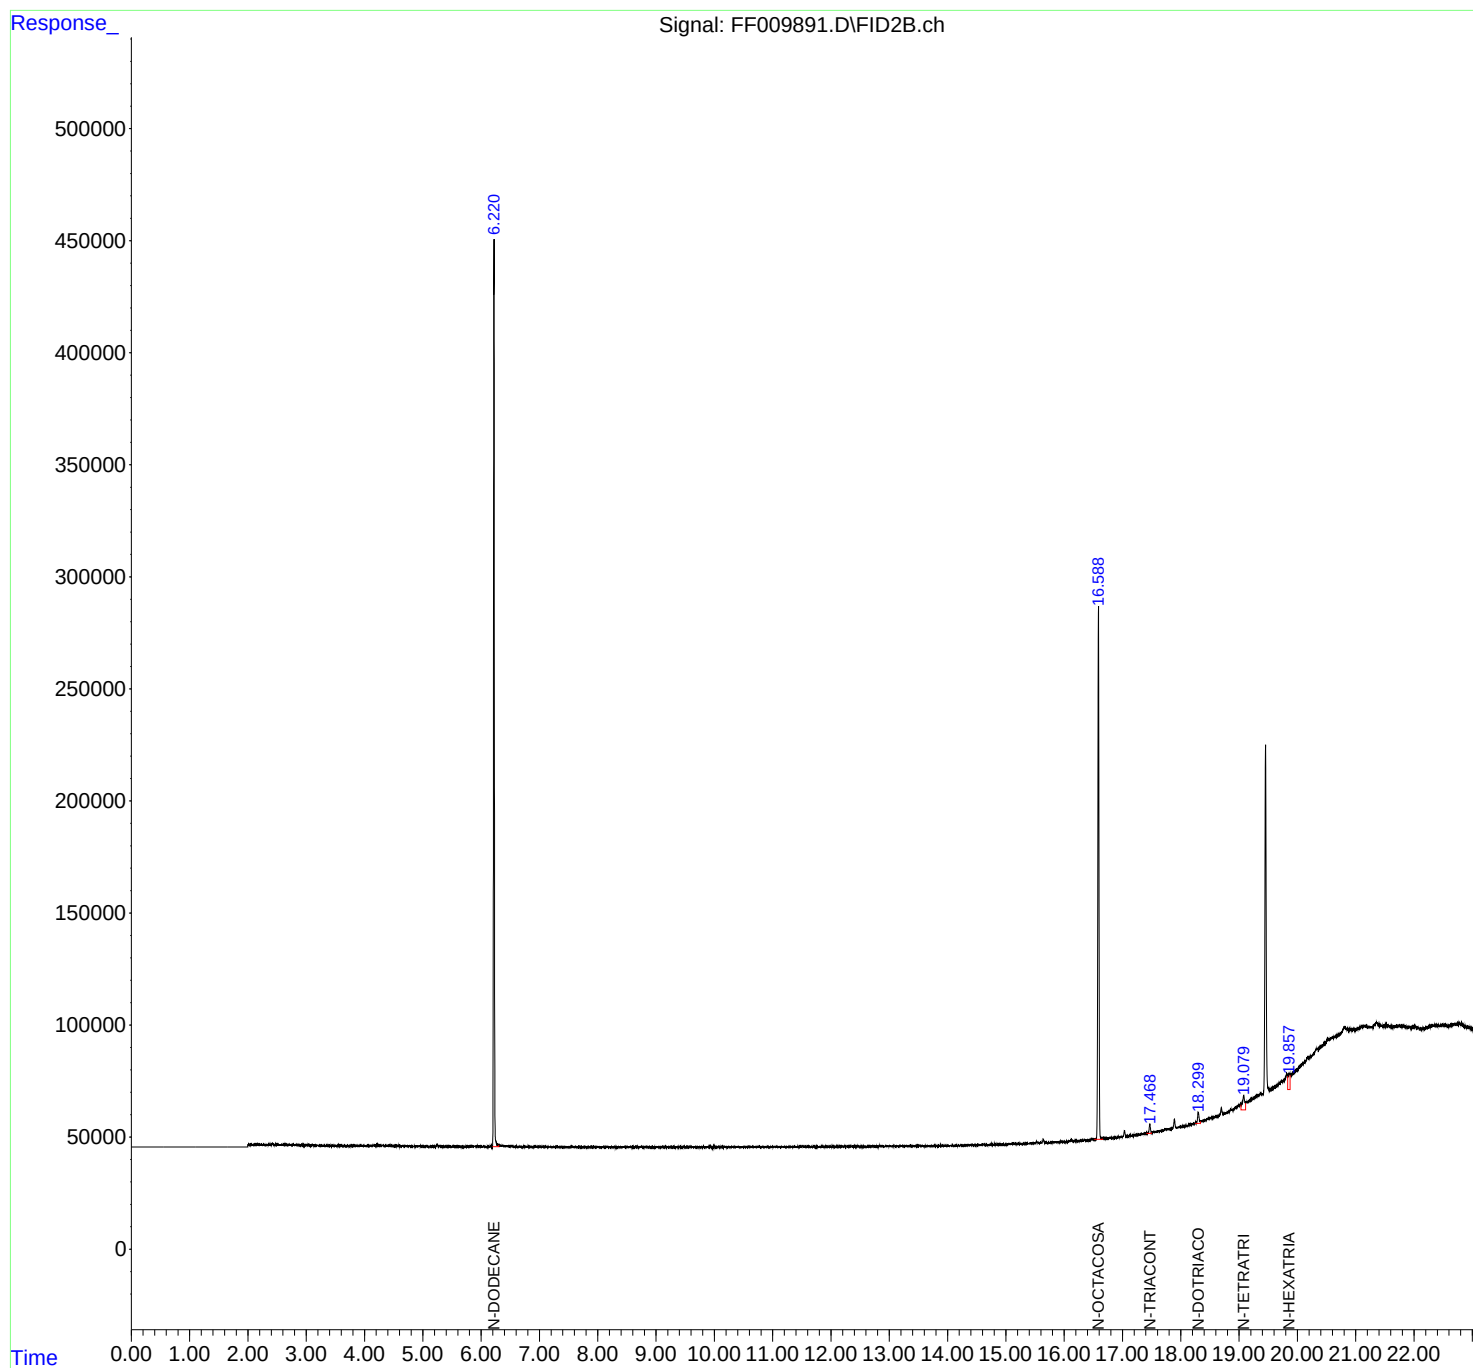


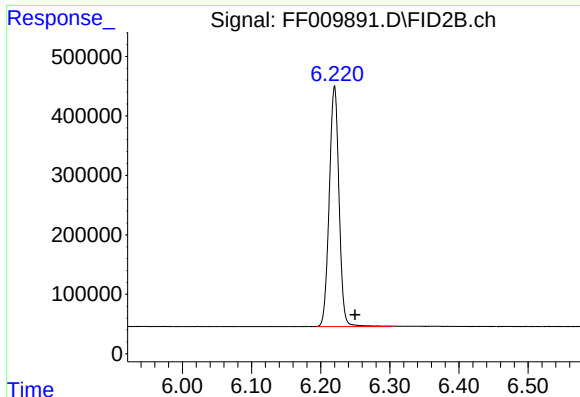

#3 N-DODECANE


R.T.: 6.220 min
Delta R.T.: -0.030 min
Response: 3979273
Conc: 27.81 ug/ml

Instrument :
FID_F
ClientSampleId :

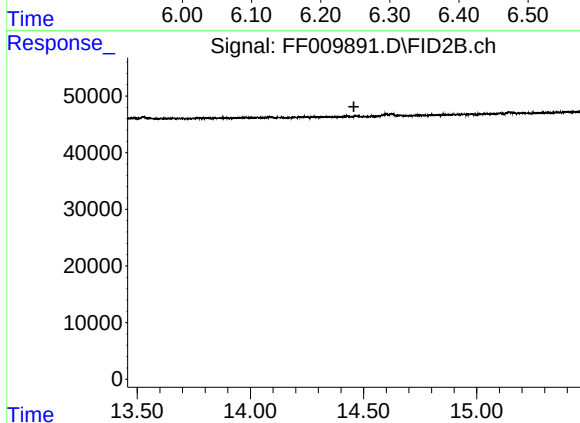


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

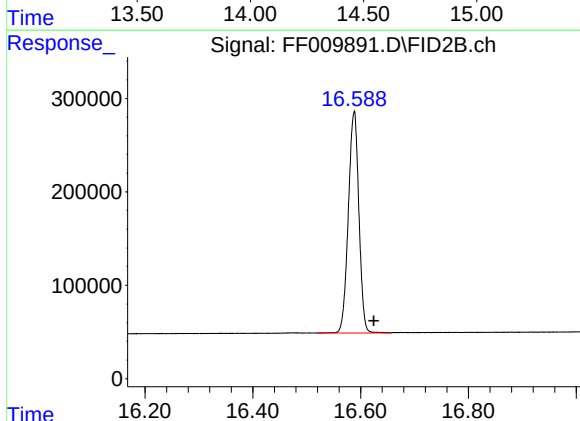


#12 N-OCTACOSANE

R.T.: 16.589 min
Delta R.T.: -0.035 min
Response: 3221547
Conc: 22.19 ug/ml

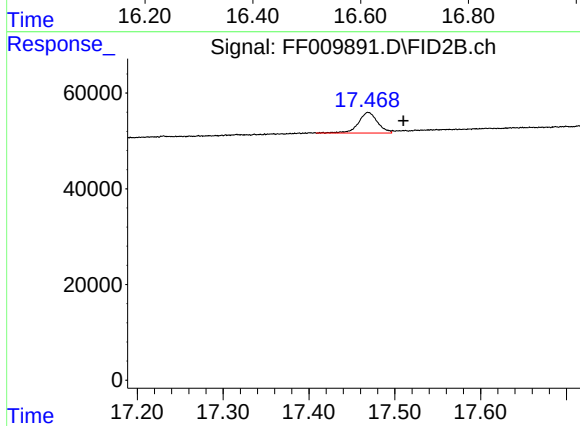

#13 N-TRIACONTANE


R.T.: 17.469 min
Delta R.T.: -0.041 min
Response: 65760
Conc: 0.46 ug/ml

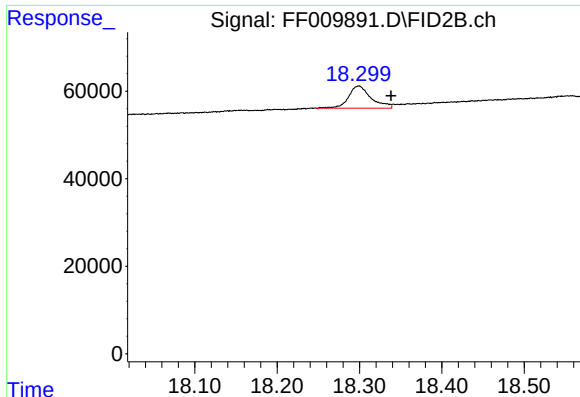

#14 N-DOTRIACONTANE


R.T.: 18.299 min
Delta R.T.: -0.039 min
Response: 96672
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

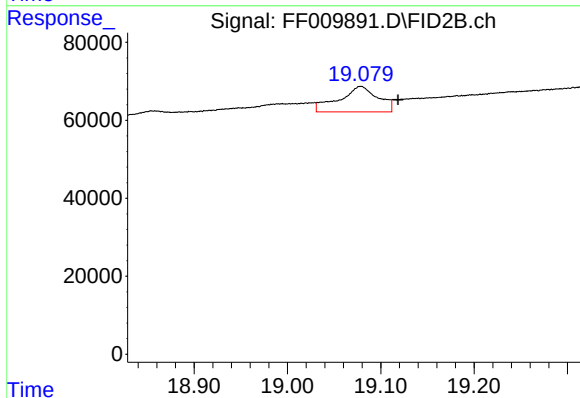

#15 N-TETRATRIACONTANE

R.T.: 19.079 min
Delta R.T.: -0.040 min
Response: 189263
Conc: 1.59 ug/ml

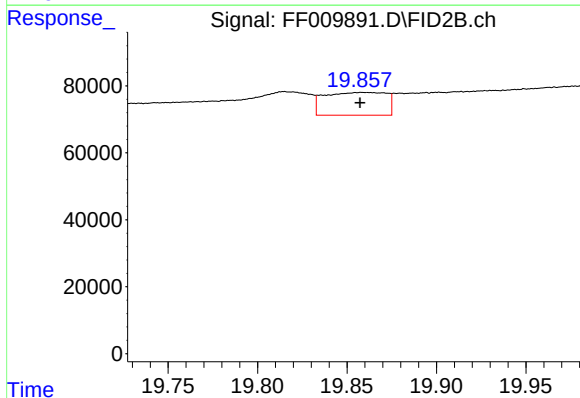

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: 0.000 min
Response: 163546
Conc: 1.59 ug/ml