

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
 Data File : FF009895.D
 Signal(s) : FID2B.ch
 Acq On : 07 Feb 2022 15:11
 Operator : AJ\MA
 Sample : N1393-04 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 08 02:57:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	614197	4.700 ug/ml
Target Compounds			
3) N-DODECANE	6.204	104651	0.731 ug/ml
4) N-TETRADECANE	8.023	68250	0.464 ug/ml
6) N-OCTADECANE	11.088	396234	2.570 ug/ml
14) N-DOTRIACONTANE	18.307	635593	4.671 ug/ml
15) N-TETRATRIACONTANE	19.077	1420257	11.958 ug/ml
16) N-HEXATRIACONTANE	19.856	605618	5.874 ug/ml
18) N-TETRACONTANE	21.356	184991	2.037 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009895.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 15:11
Operator : AJ\MA
Sample : N1393-04 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:57:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

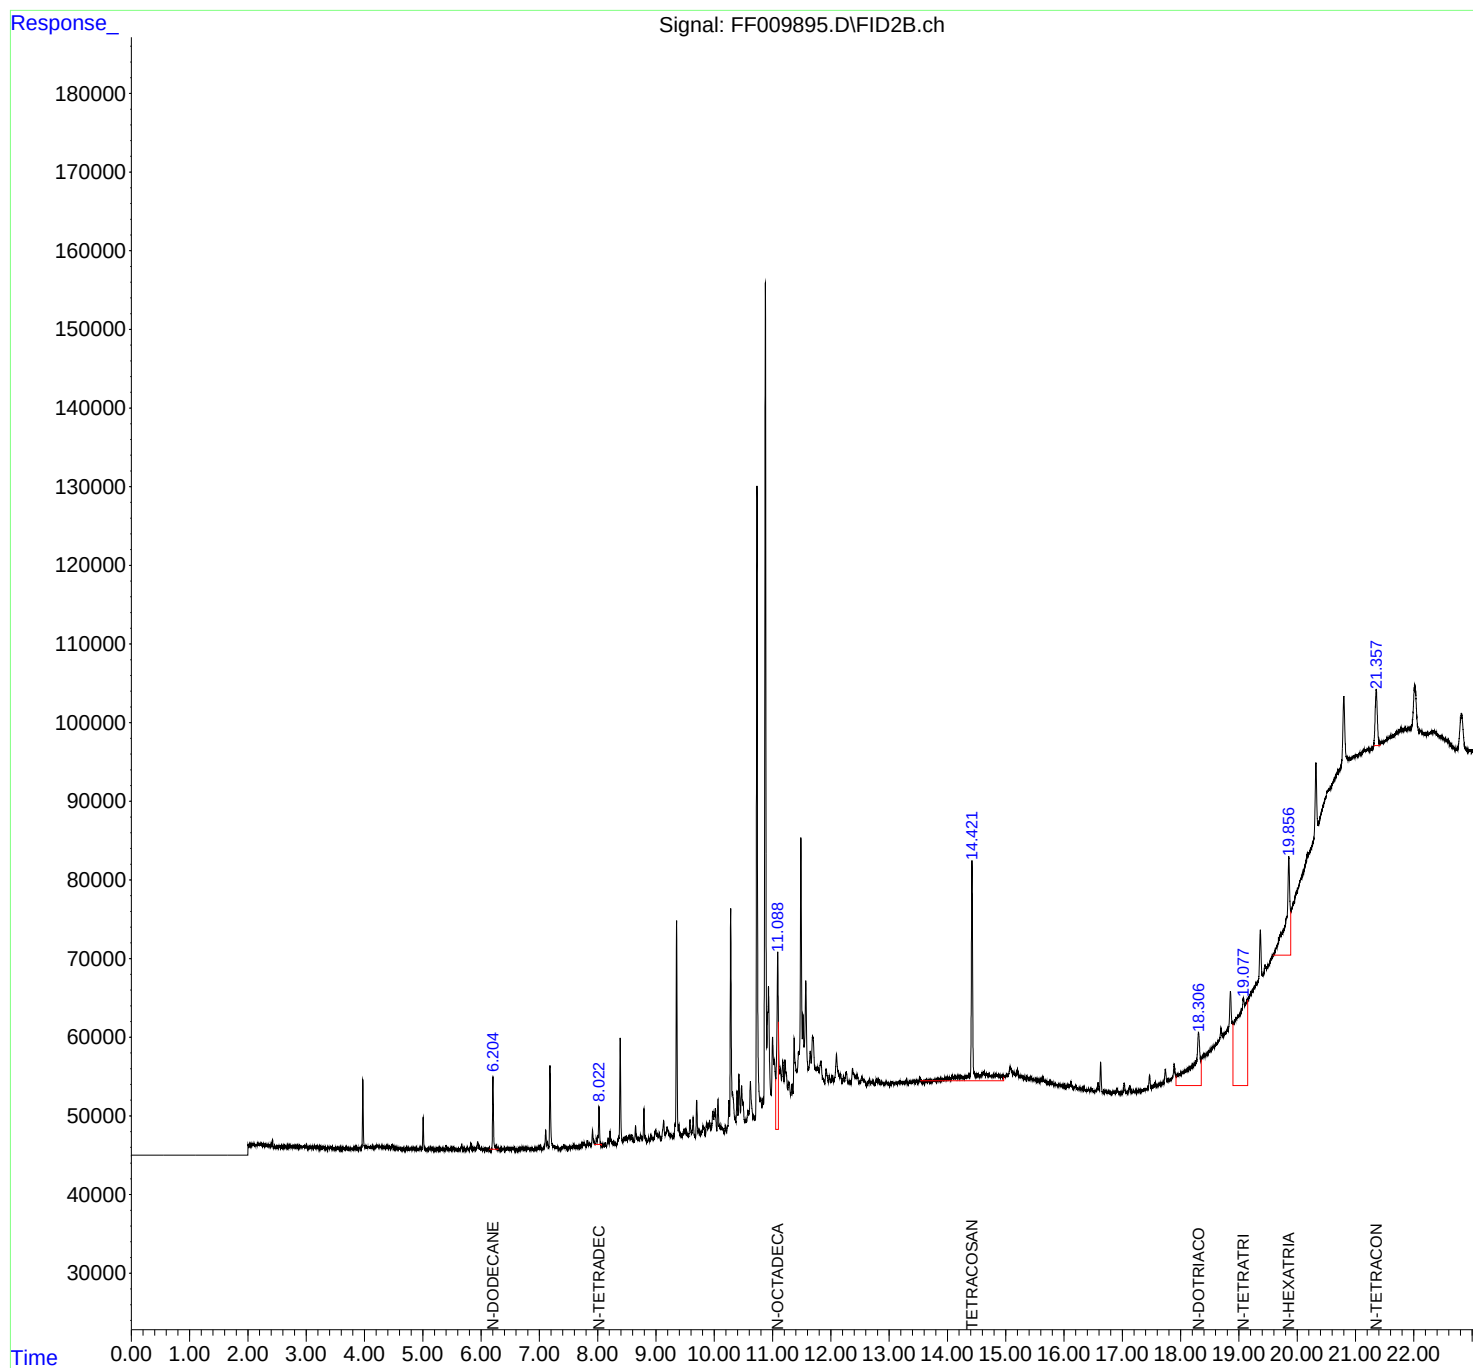


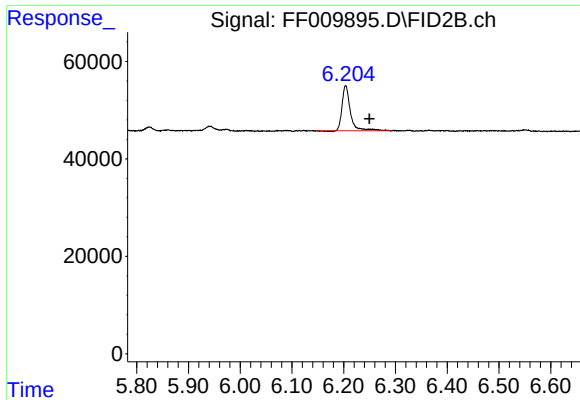

#3 N-DODECANE


R.T.: 6.204 min
Delta R.T.: -0.046 min
Response: 104651
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :

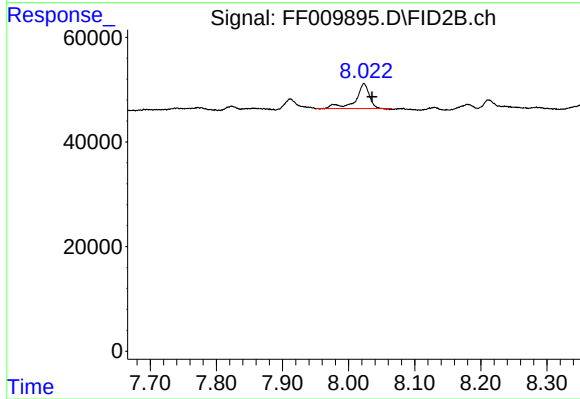


#4 N-TETRADECANE

R.T.: 8.023 min
Delta R.T.: -0.012 min
Response: 68250
Conc: 0.46 ug/ml

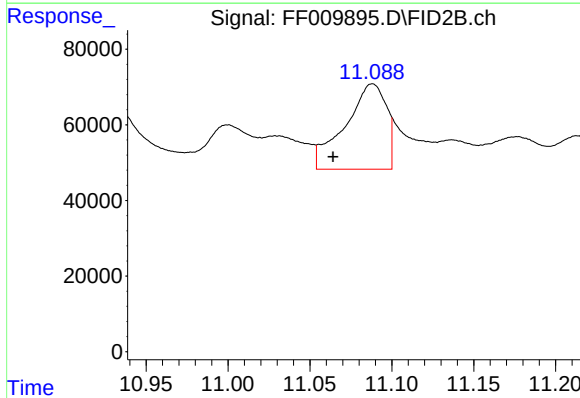


#6 N-OCTADECANE

R.T.: 11.088 min
Delta R.T.: 0.024 min
Response: 396234
Conc: 2.57 ug/ml

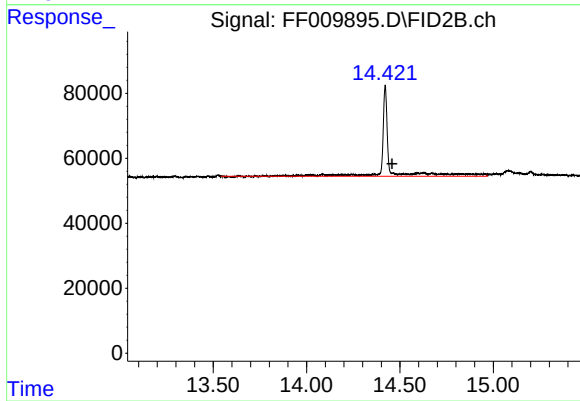

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.421 min
Delta R.T.: -0.036 min
Response: 614197
Conc: 4.70 ug/ml

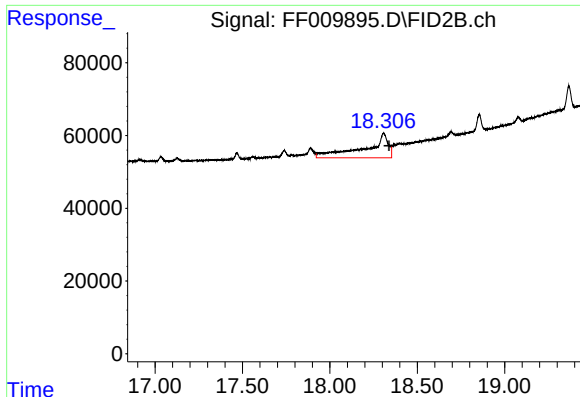

#14 N-DOTRIACONTANE


R.T.: 18.307 min
Delta R.T.: -0.032 min
Response: 635593
Conc: 4.67 ug/ml

Instrument :
FID_F
ClientSampleId :

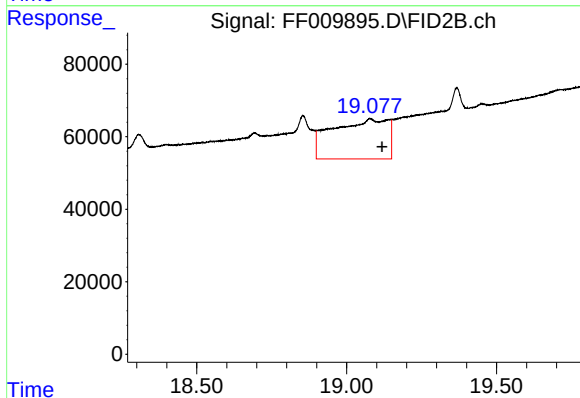


#15 N-TETRATRIACONTANE

R.T.: 19.077 min
Delta R.T.: -0.042 min
Response: 1420257
Conc: 11.96 ug/ml

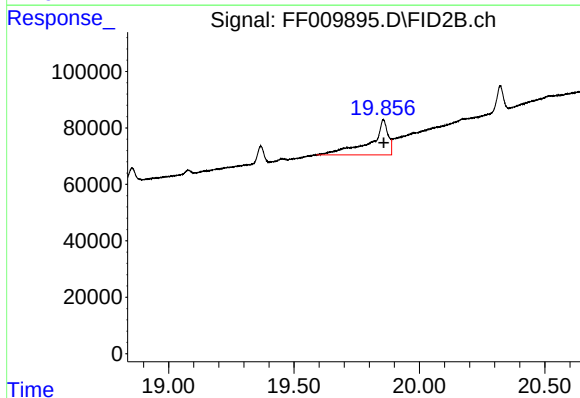

#16 N-HEXATRIACONTANE

R.T.: 19.856 min
Delta R.T.: -0.001 min
Response: 605618
Conc: 5.87 ug/ml

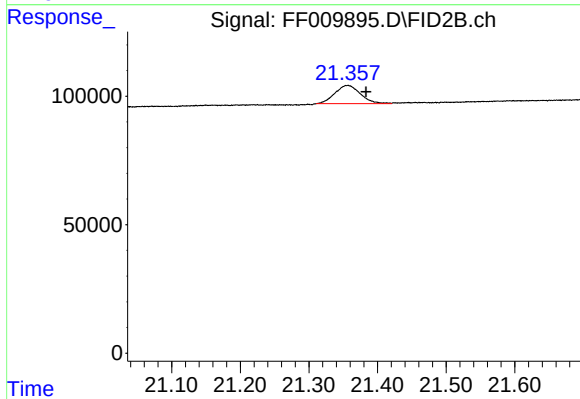

#18 N-TETRACONTANE

R.T.: 21.356 min
Delta R.T.: -0.027 min
Response: 184991
Conc: 2.04 ug/ml