

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009896.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 15:40
Operator : AJ\MA
Sample : N1397-03 50X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:57:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.297	70211	0.516 ug/ml
16) N-HEXATRIACONTANE	19.858	94198	0.914 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009896.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 15:40
Operator : AJ\MA
Sample : N1397-03 50X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:57:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

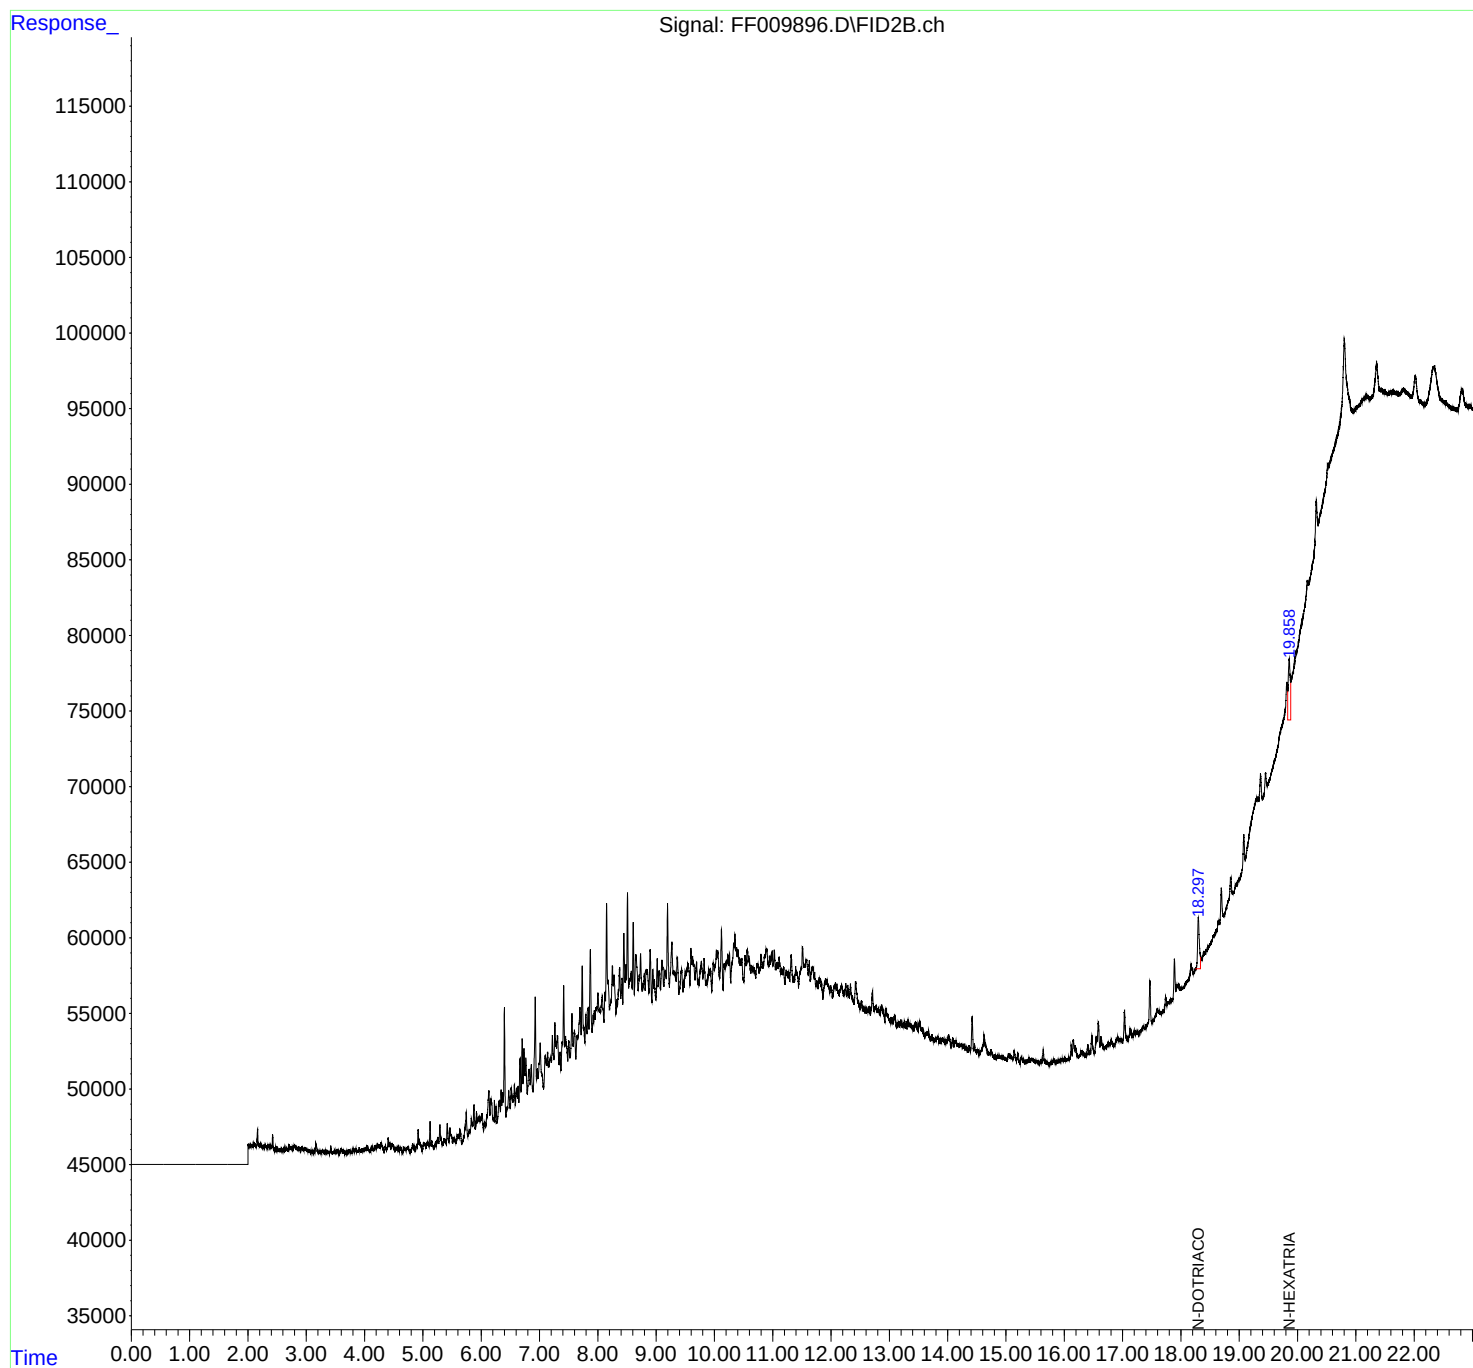


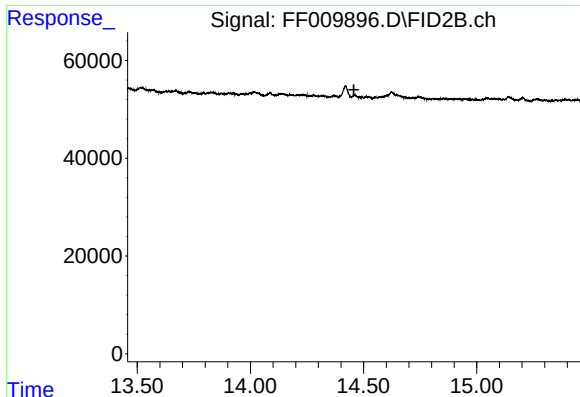

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

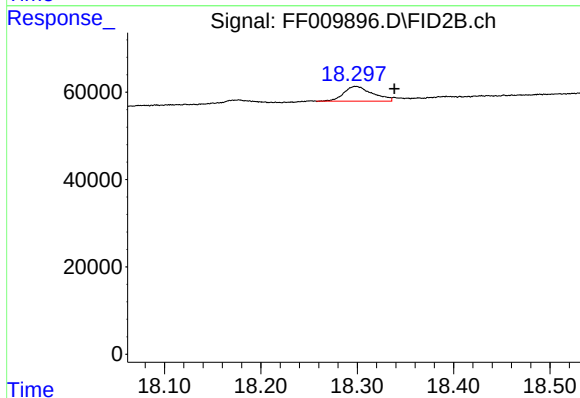

#14 N-DOTRIACONTANE

R.T.: 18.297 min
Delta R.T.: -0.041 min
Response: 70211
Conc: 0.52 ug/ml

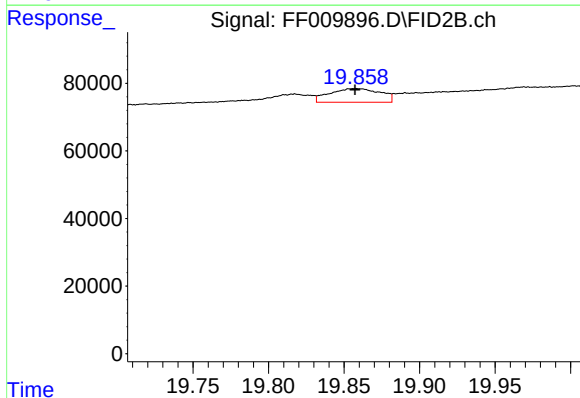

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: 0.001 min
Response: 94198
Conc: 0.91 ug/ml