

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009898.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 16:40
Operator : AJ\MA
Sample : N1400-01 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16)	N-HEXATRIACONTANE	19.857	91572	0.888 ug/ml
-----	-------------------	--------	-------	-------------

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009898.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 16:40
Operator : AJ\MA
Sample : N1400-01 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 02:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

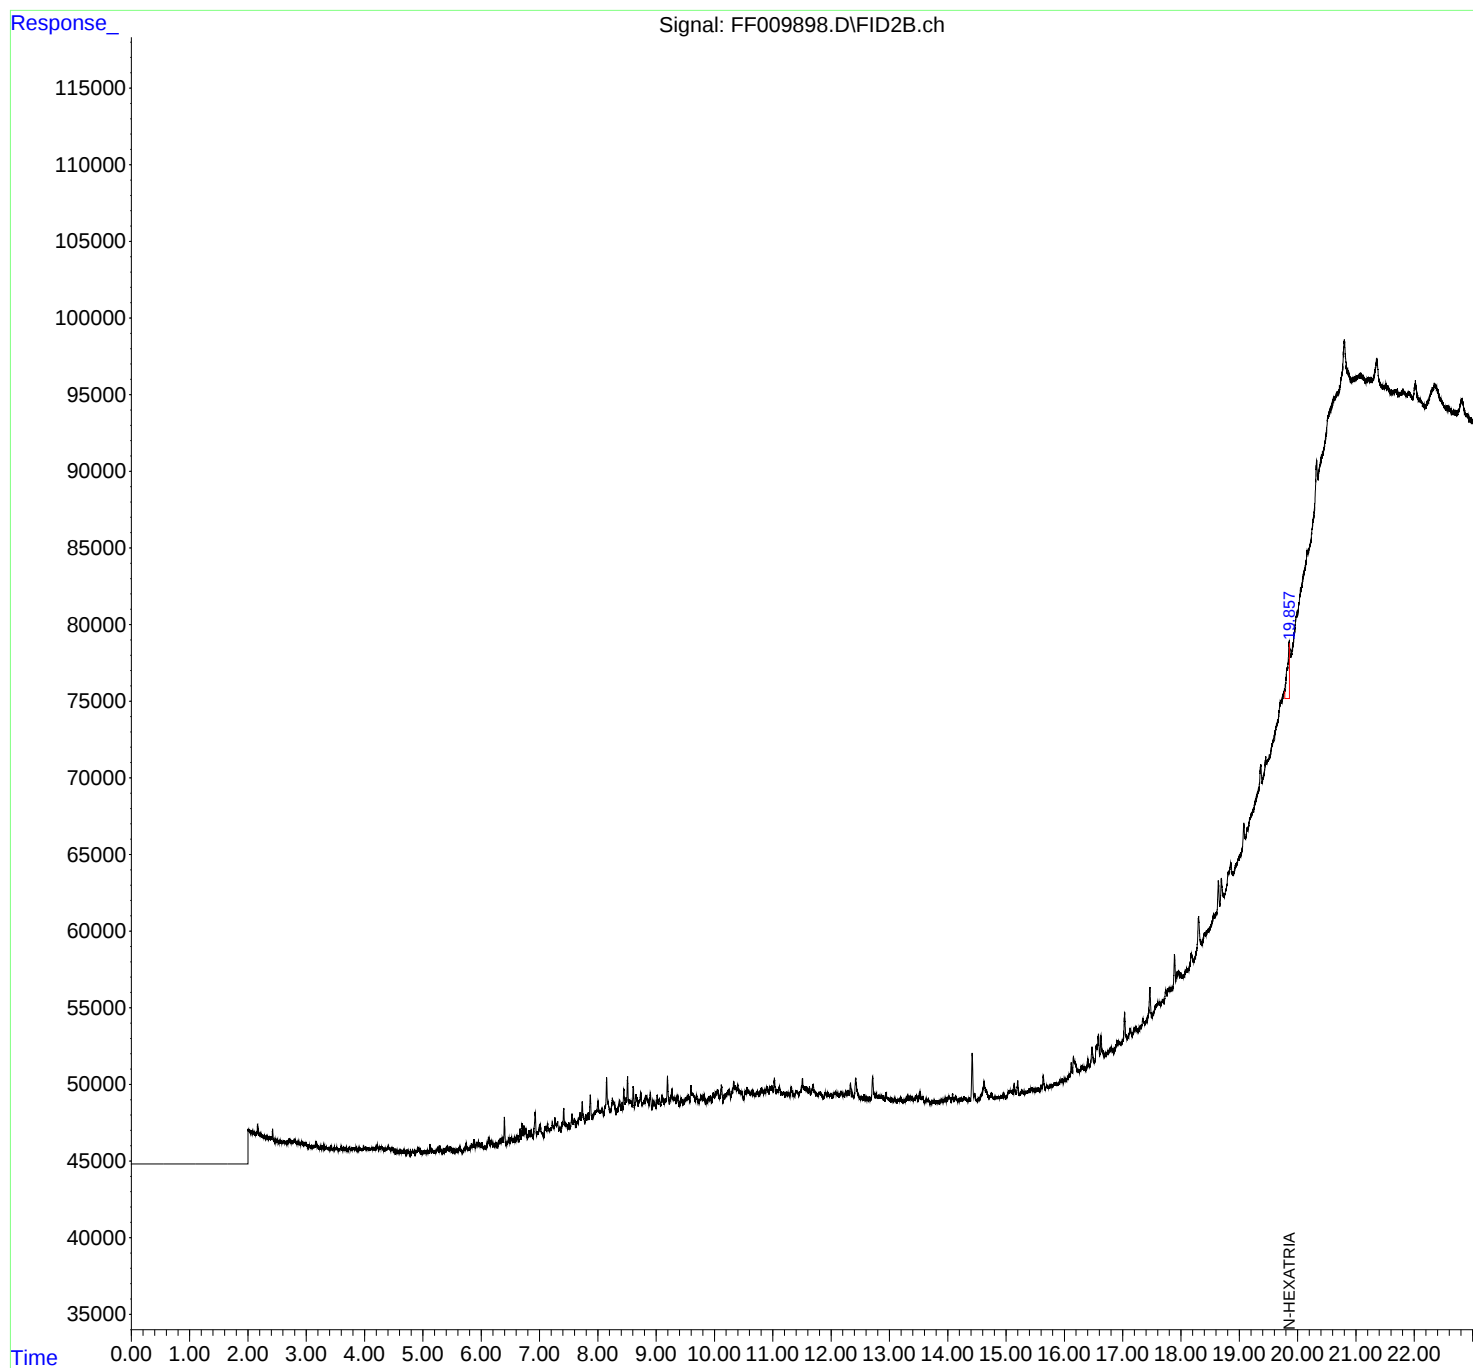


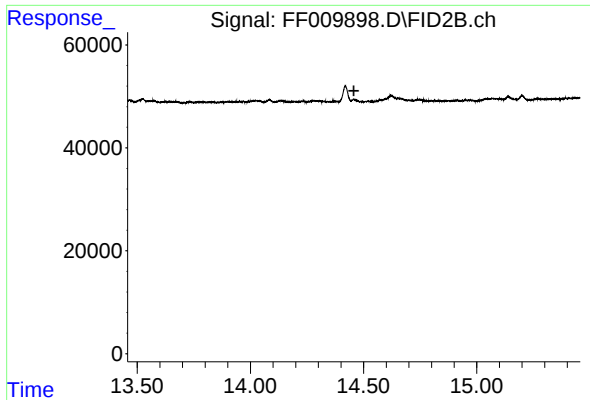

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

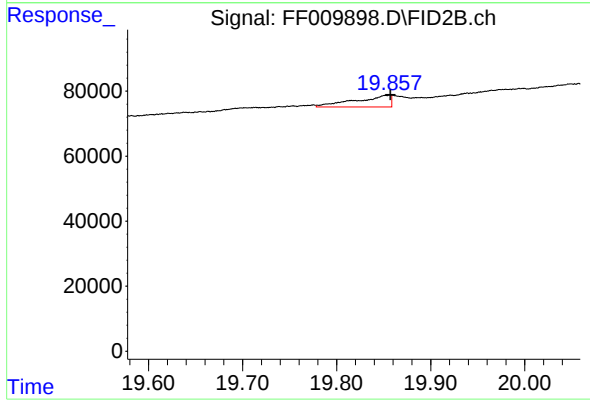

#16 N-HEXATRIACONTANE

R.T.: 19.857 min
Delta R.T.: 0.000 min
Response: 91572
Conc: 0.89 ug/ml