

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
 Data File : FF009895.D
 Signal(s) : FID2B.ch
 Acq On : 07 Feb 2022 15:11
 Operator : AJ\MA
 Sample : N1393-04 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP25-03-20220203-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/08/2022
 Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
 Quant Time: Feb 08 02:57:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	384995	2.946 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009895.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 15:11
Operator : AJ\MA
Sample : N1393-04 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SP25-03-20220203-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
Quant Time: Feb 08 02:57:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

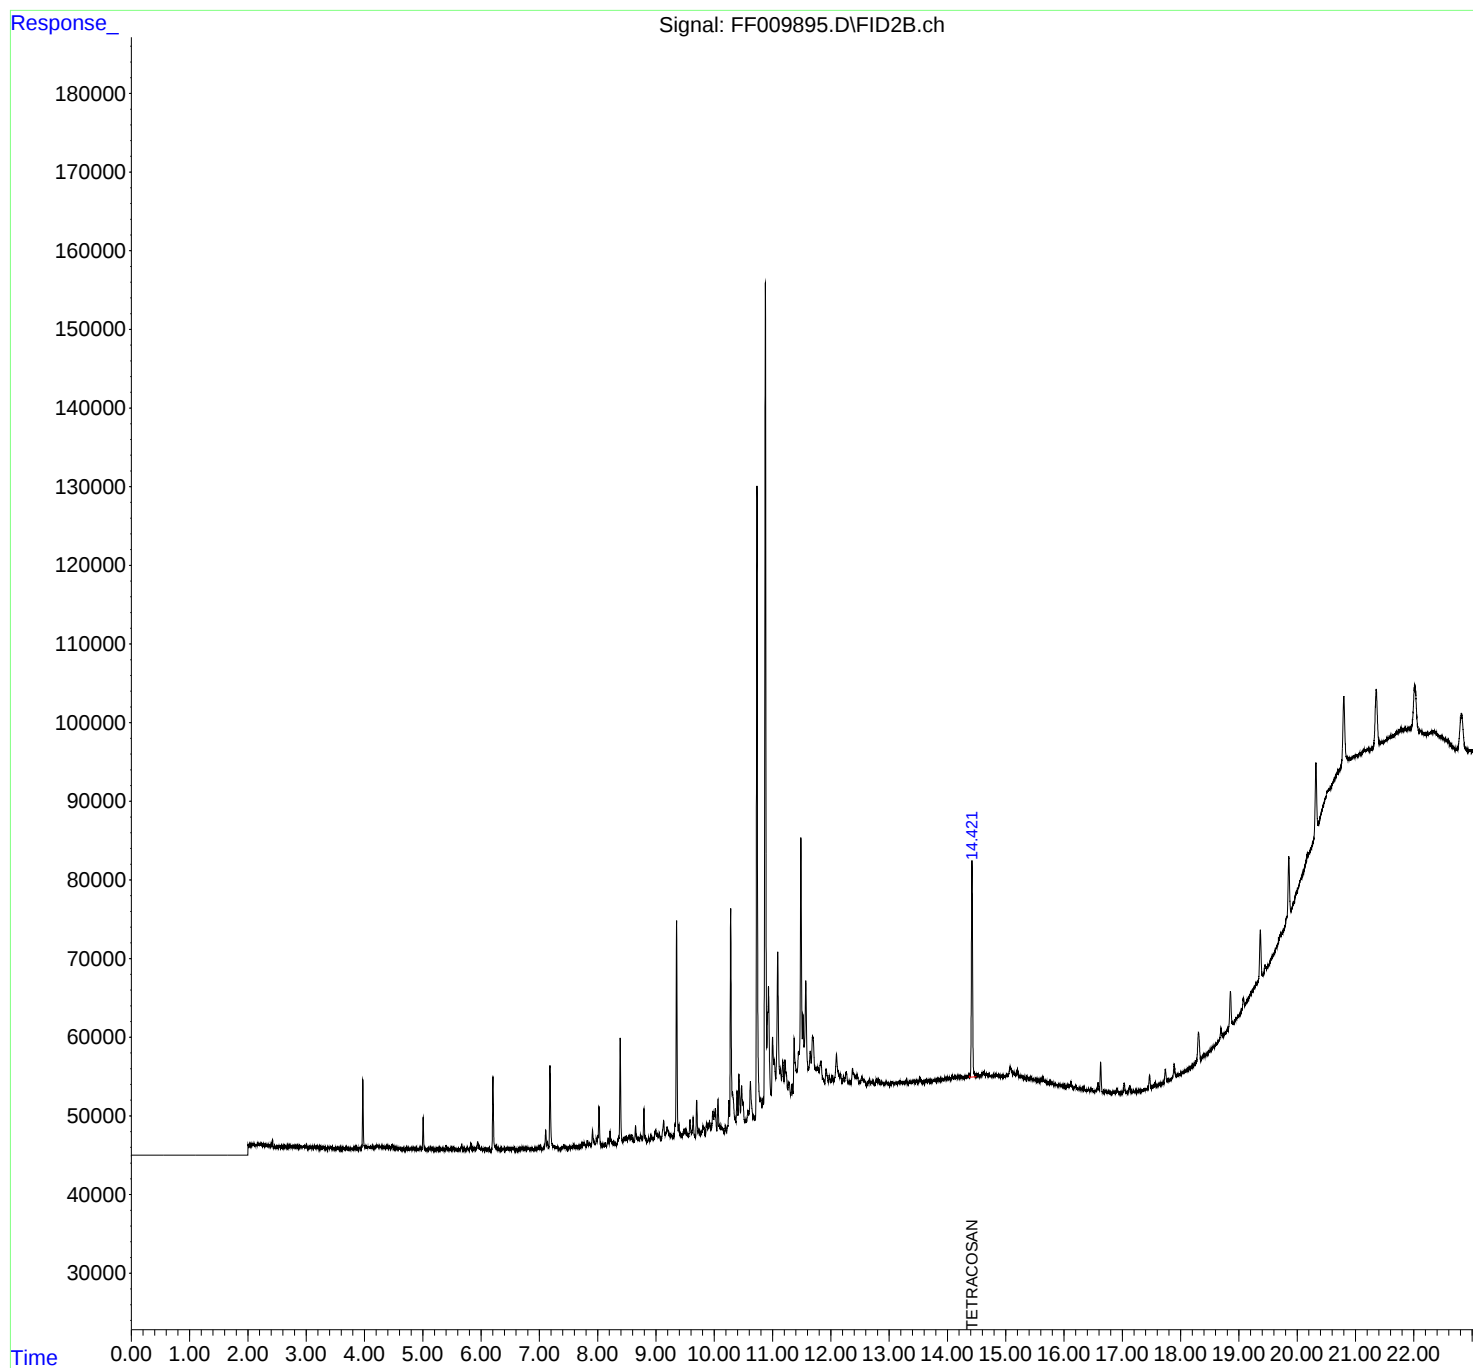

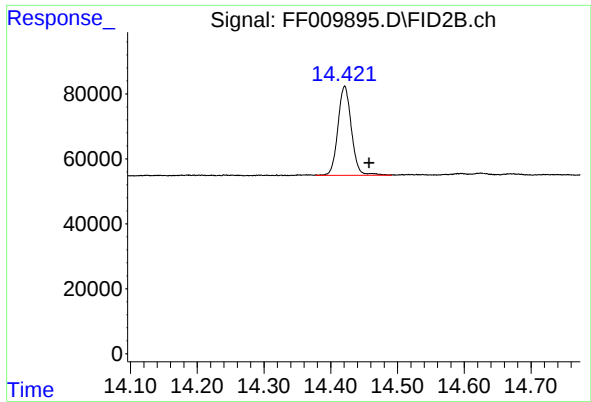

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.037 min
Response: 384995
Conc: 2.95 ug/ml

Instrument :
FID_F
ClientSampleId :
SP25-03-20220203-A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022