

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009898.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 16:40
Operator : AJ\MA
Sample : N1400-01 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTSI-WC-S-MH-01-02-0-15

Integration File: calibration.e
Quant Time: Feb 08 02:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009898.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 16:40
Operator : AJ\MA
Sample : N1400-01 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTSI-WC-S-MH-01-02-0-15

Integration File: calibration.e
Quant Time: Feb 08 02:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

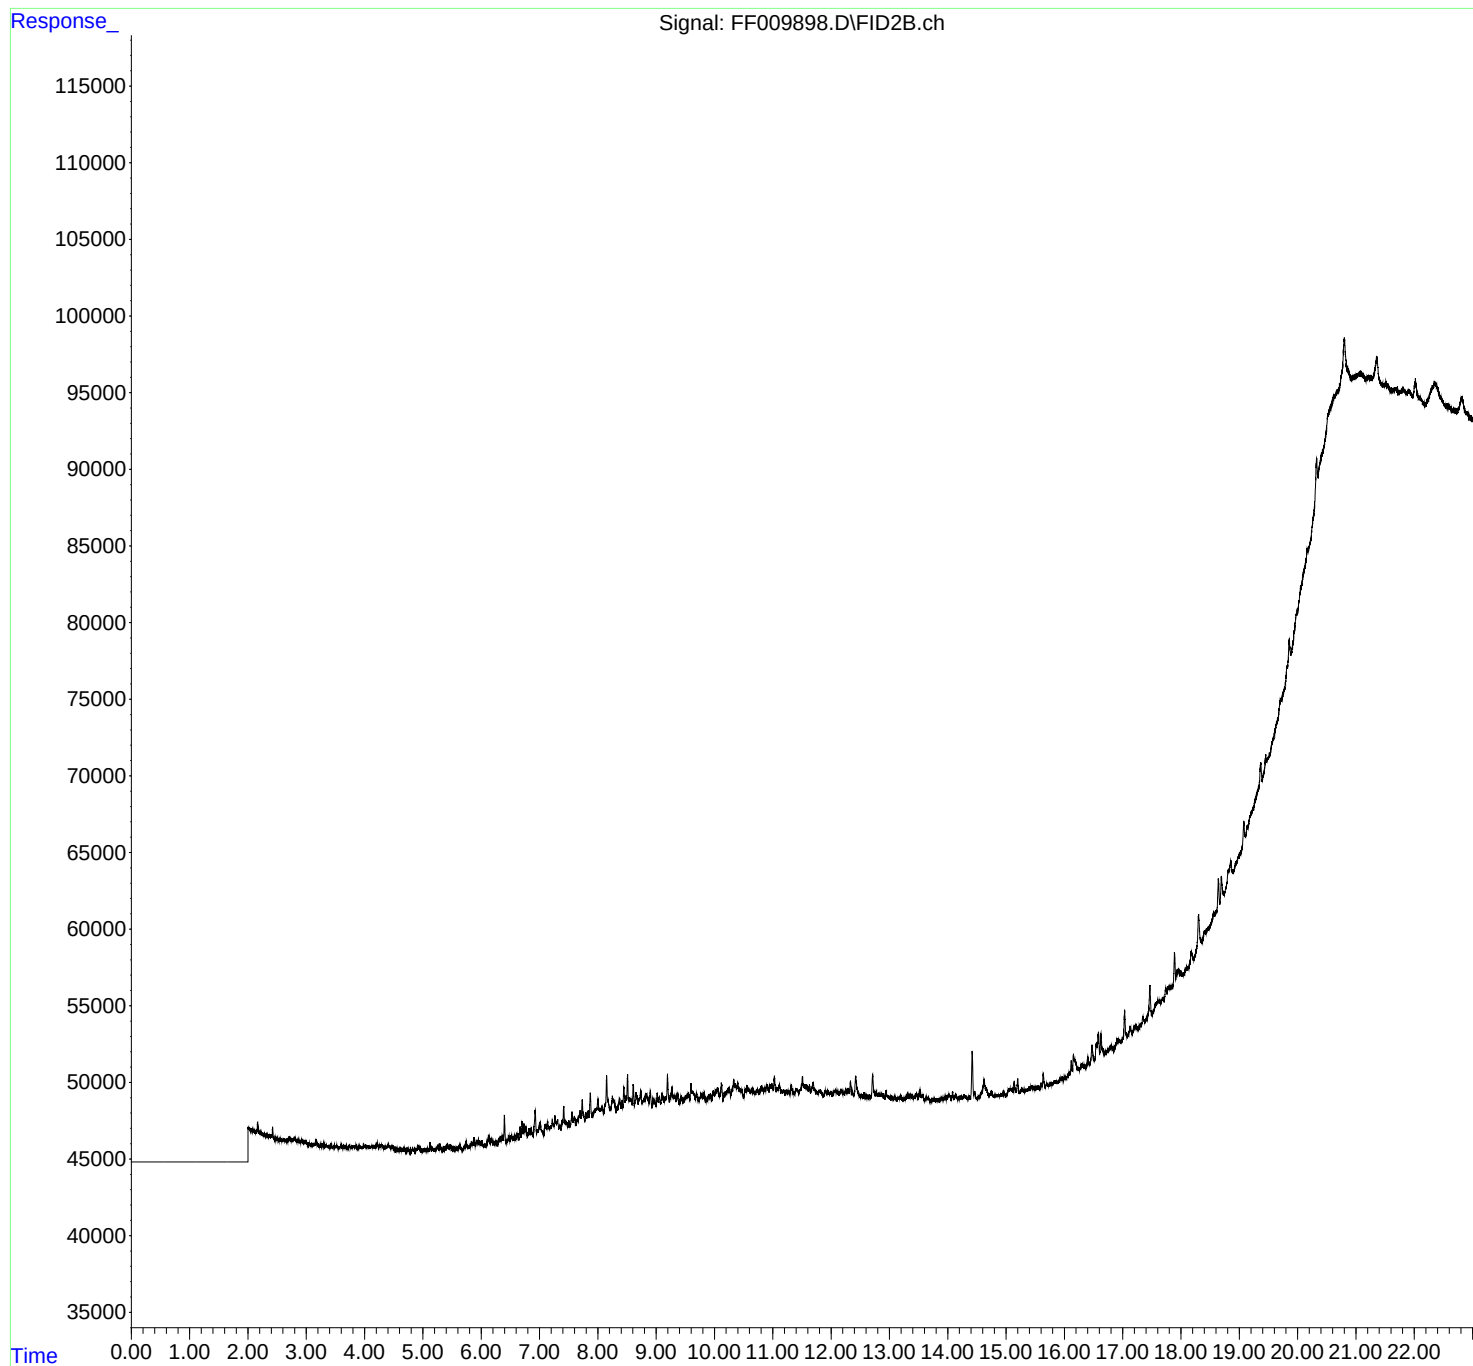

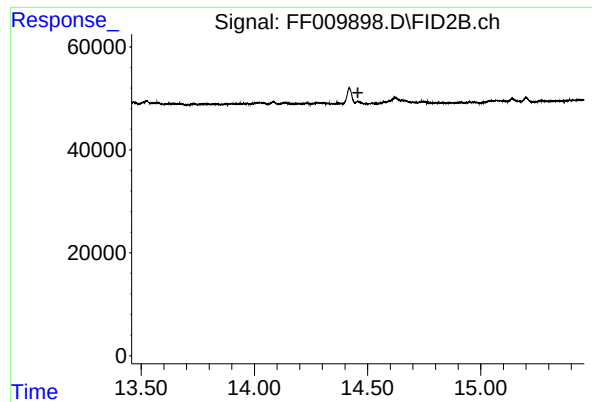

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
KTSI-WC-S-MH-01-02-0-15