

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009900.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 17:39
Operator : AJ\MA
Sample : N1400-02 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS1-WC-L-MH-02

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
Quant Time: Feb 08 02:58:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.419	265469	2.031 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009900.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 17:39
Operator : AJ\MA
Sample : N1400-02 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
KTS1-WC-L-MH-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
Quant Time: Feb 08 02:58:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

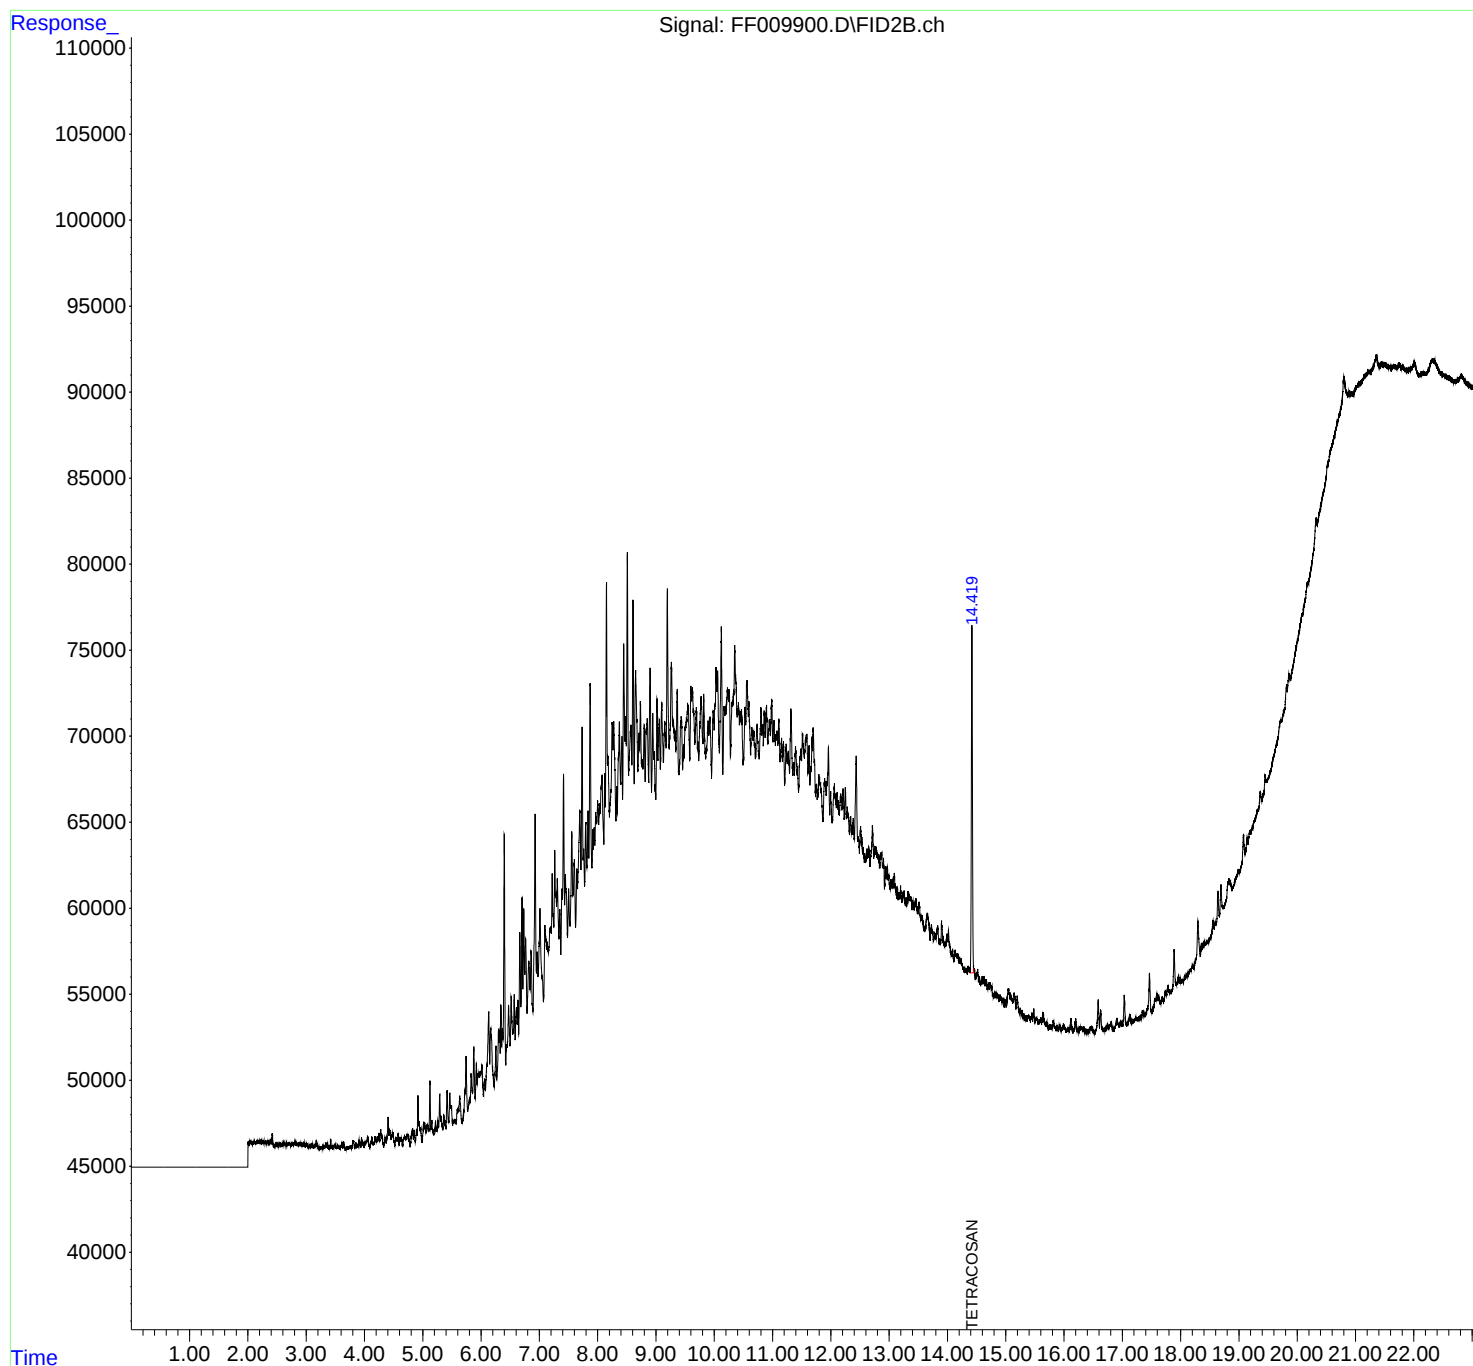

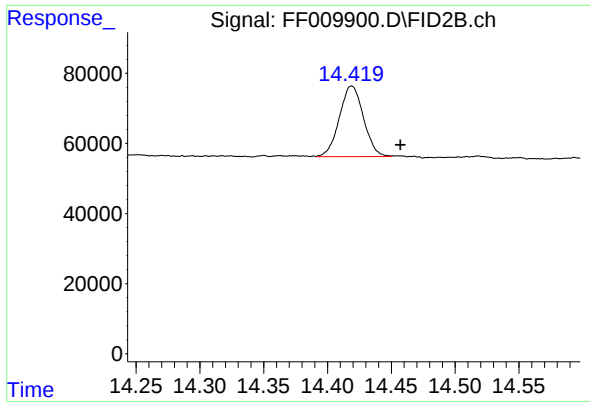

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.419 min
Delta R.T.: -0.038 min
Response: 265469
Conc: 2.03 ug/ml

Instrument :

FID_F

ClientSampleId :

KTS1-WC-L-MH-02

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022