

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009909.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 22:34
Operator : AJ\MA
Sample : N1424-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DB-10(13-15)-02-04-22

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
Quant Time: Feb 08 02:59:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	2035566	15.577 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020722\
Data File : FF009909.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2022 22:34
Operator : AJ\MA
Sample : N1424-01
Misc :
ALS Vial : 71 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
DB-10(13-15)-02-04-22


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022

Integration File: calibration.e
Quant Time: Feb 08 02:59:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

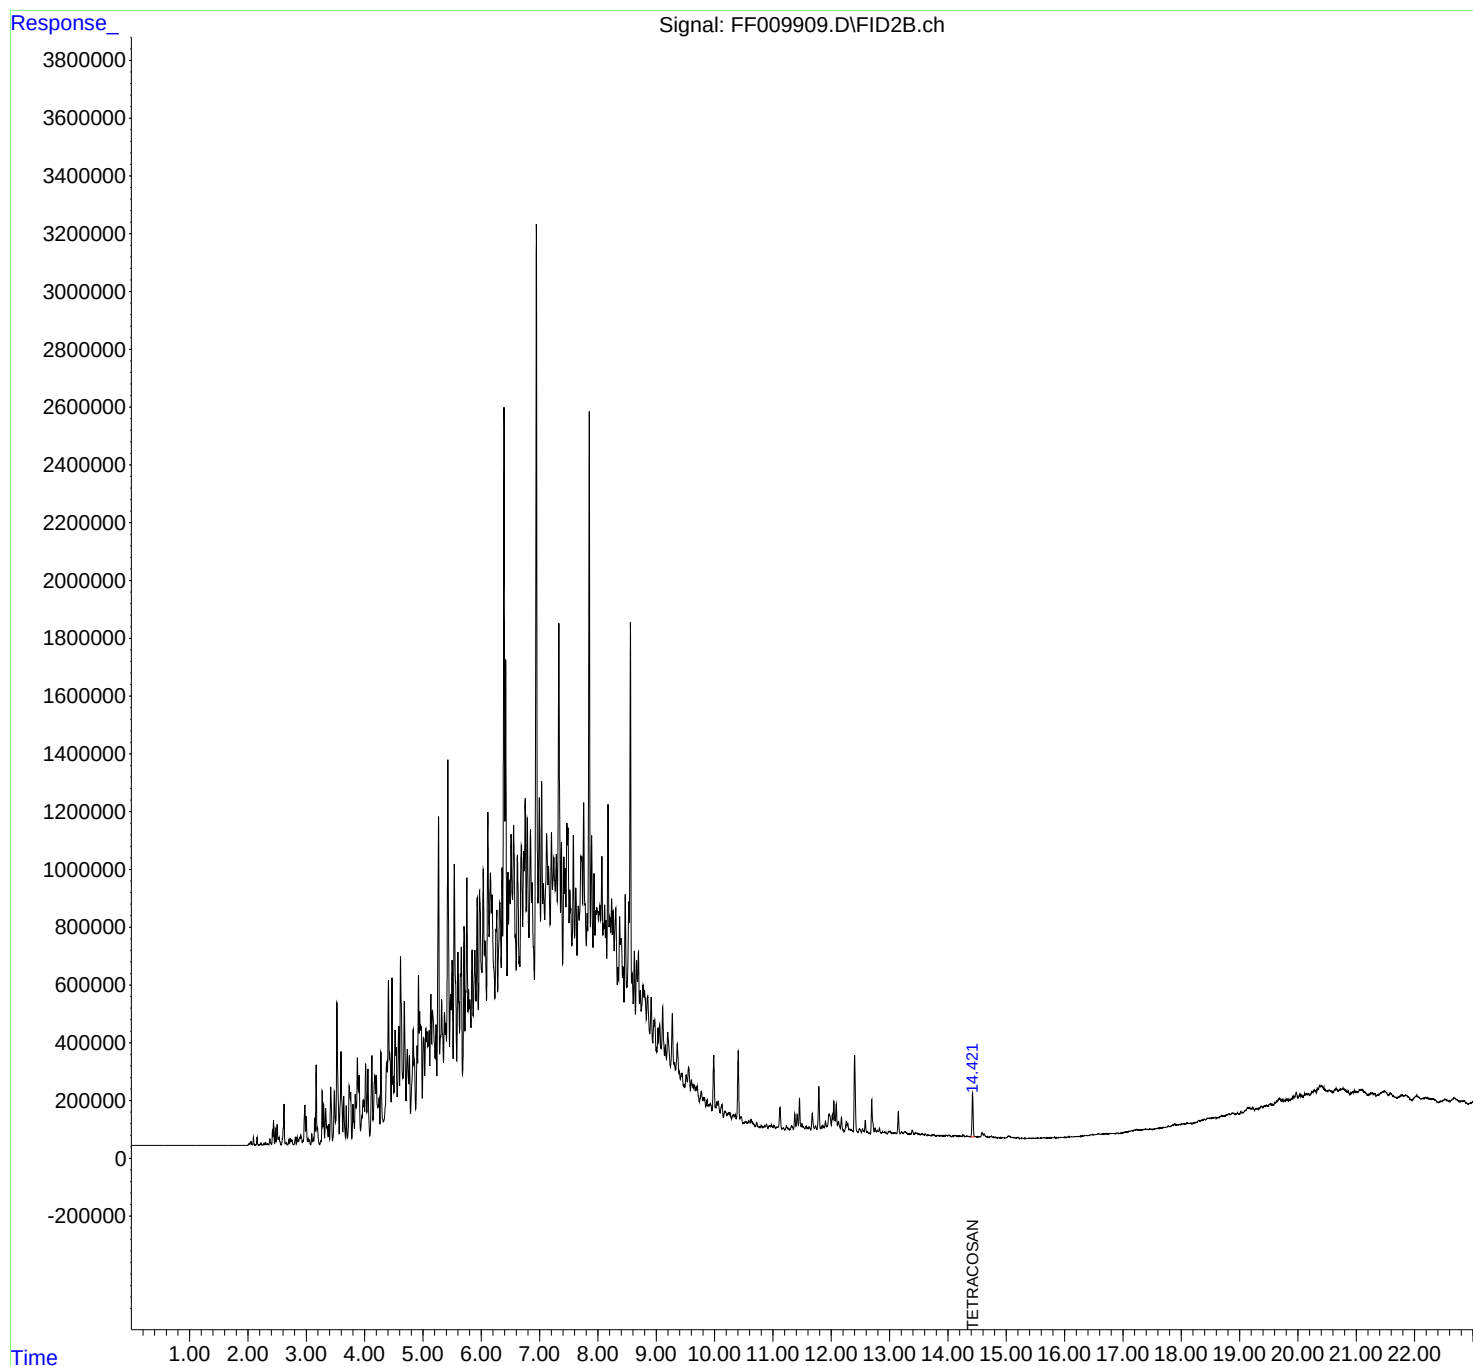

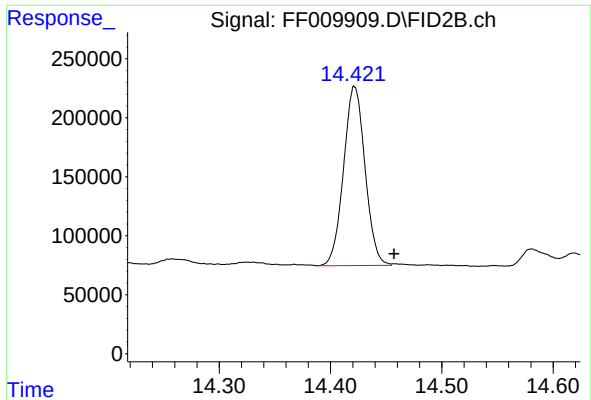

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.037 min
Response: 2035566
Conc: 15.58 ug/ml

Instrument : FID_F
ClientSampleId : DB-10(13-15)-02-04-22

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/08/2022
Supervised By :Ankita Jodhani 02/08/2022