

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
Data File : FF011996.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2023 11:26
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 00:17:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.939	79277	0.609 ug/ml
16) N-HEXATRIACONTANE	20.496	58909	0.573 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
Data File : FF011996.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2023 11:26
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 00:17:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

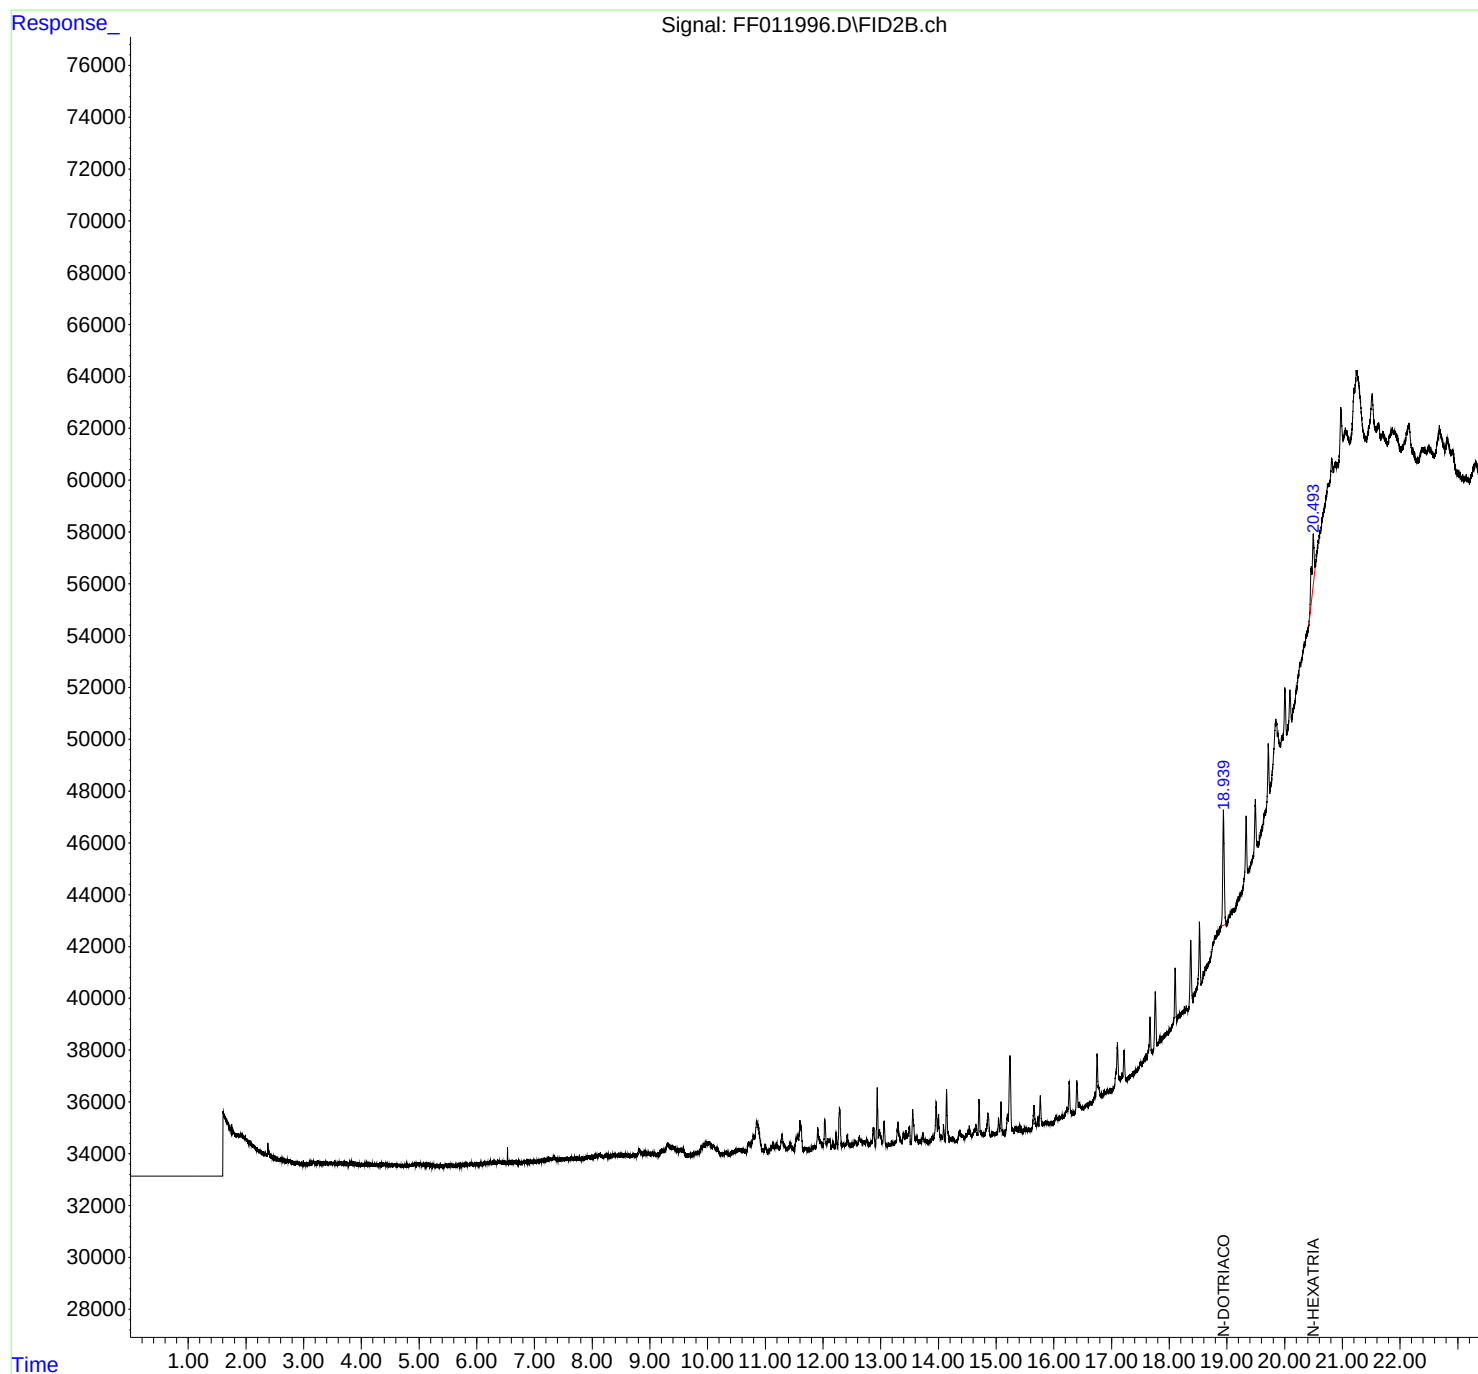


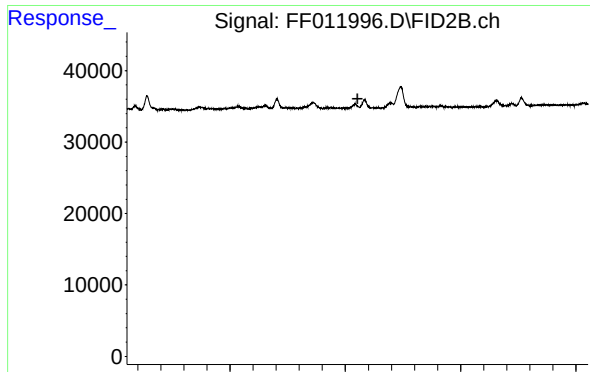

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

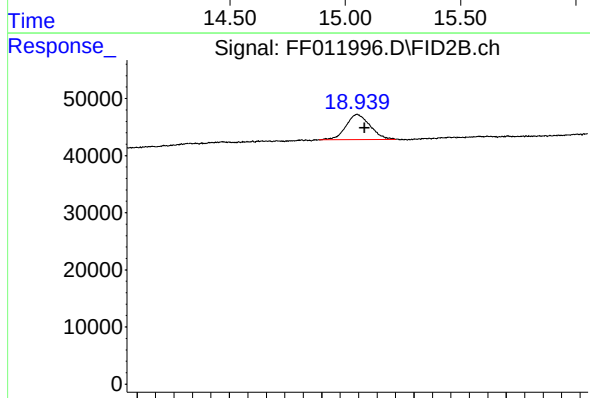

#14 N-DOTRIACONTANE

R.T.: 18.939 min
Delta R.T.: -0.008 min
Response: 79277
Conc: 0.61 ug/ml

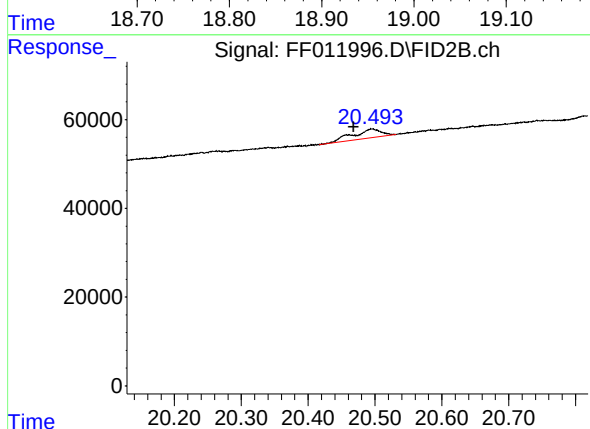

#16 N-HEXATRIACONTANE

R.T.: 20.496 min
Delta R.T.: 0.028 min
Response: 58909
Conc: 0.57 ug/ml