

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
Data File : FF011997.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2023 11:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 00:17:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.044	1813223	15.735 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.497	51450	0.501 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
Data File : FF011997.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2023 11:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 00:17:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

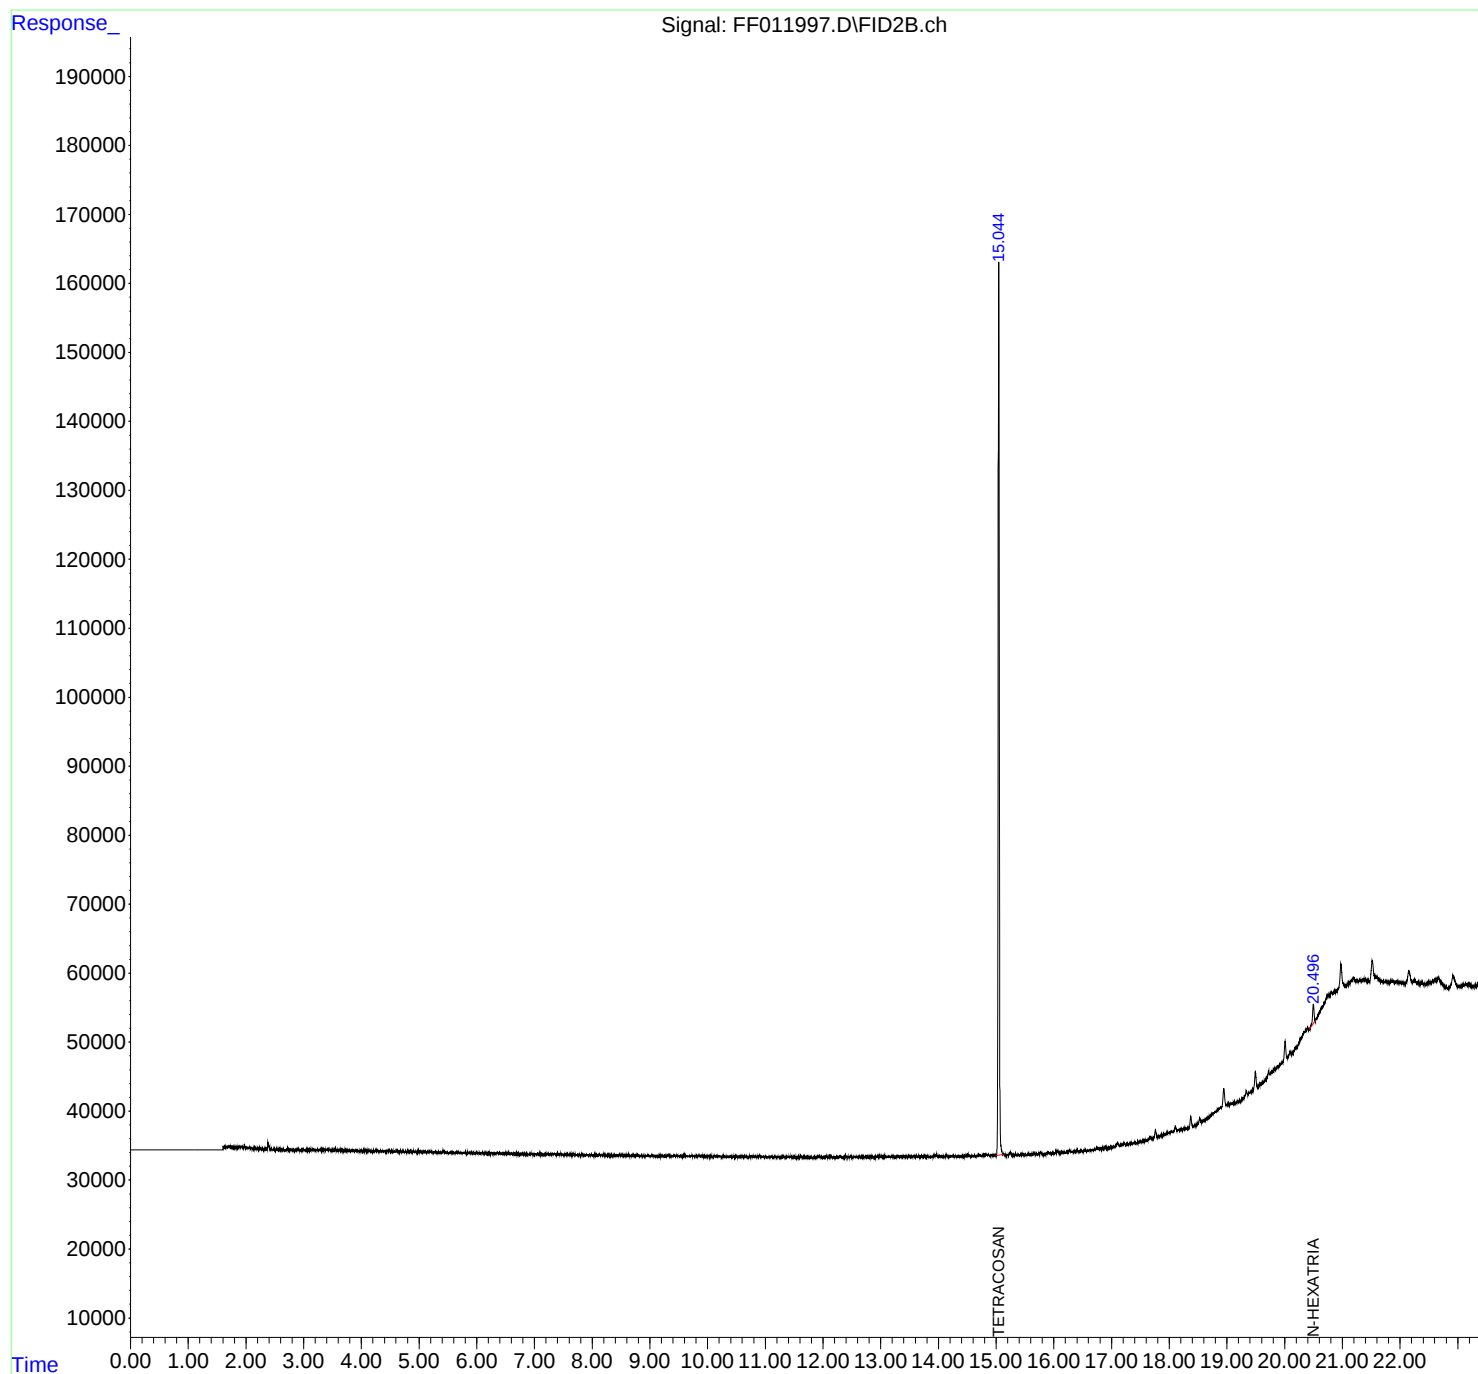


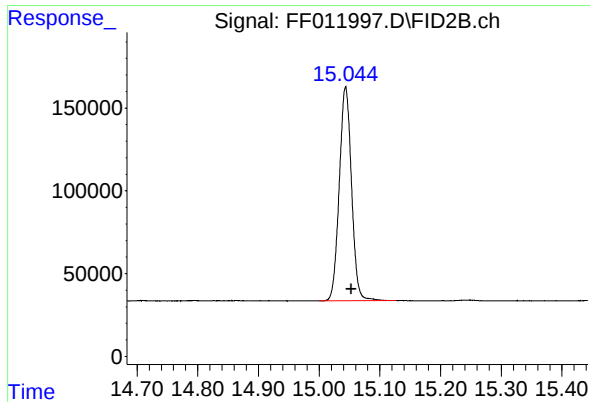

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.044 min
Delta R.T.: -0.009 min
Response: 1813223
Conc: 15.74 ug/ml

Instrument :
FID_F
ClientSampleId :

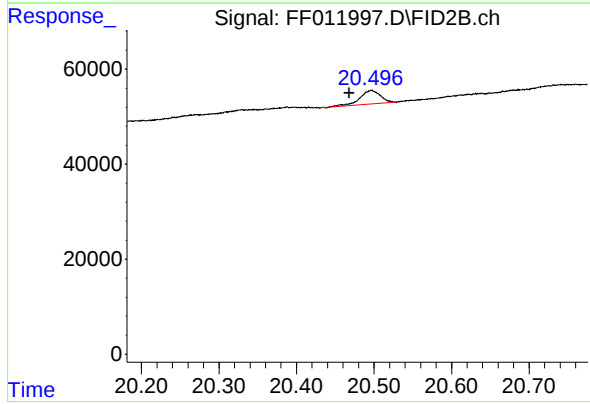

#16 N-HEXATRIACONTANE

R.T.: 20.497 min
Delta R.T.: 0.029 min
Response: 51450
Conc: 0.50 ug/ml