

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
 Data File : FF011999.D
 Signal(s) : FID2B.ch
 Acq On : 07 Feb 2023 12:58
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 08 00:17:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.762	2428706	20.275 ug/ml
12) N-OCTACOSANE	17.219	2360662	18.154 ug/ml
13) N-TRIACONTANE	18.104	47058	0.365 ug/ml
14) N-DOTRIACONTANE	18.938	93810	0.721 ug/ml
15) N-TETRATRIACONTANE	19.719	65700	0.590 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020723\
Data File : FF011999.D
Signal(s) : FID2B.ch
Acq On : 07 Feb 2023 12:58
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 00:17:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

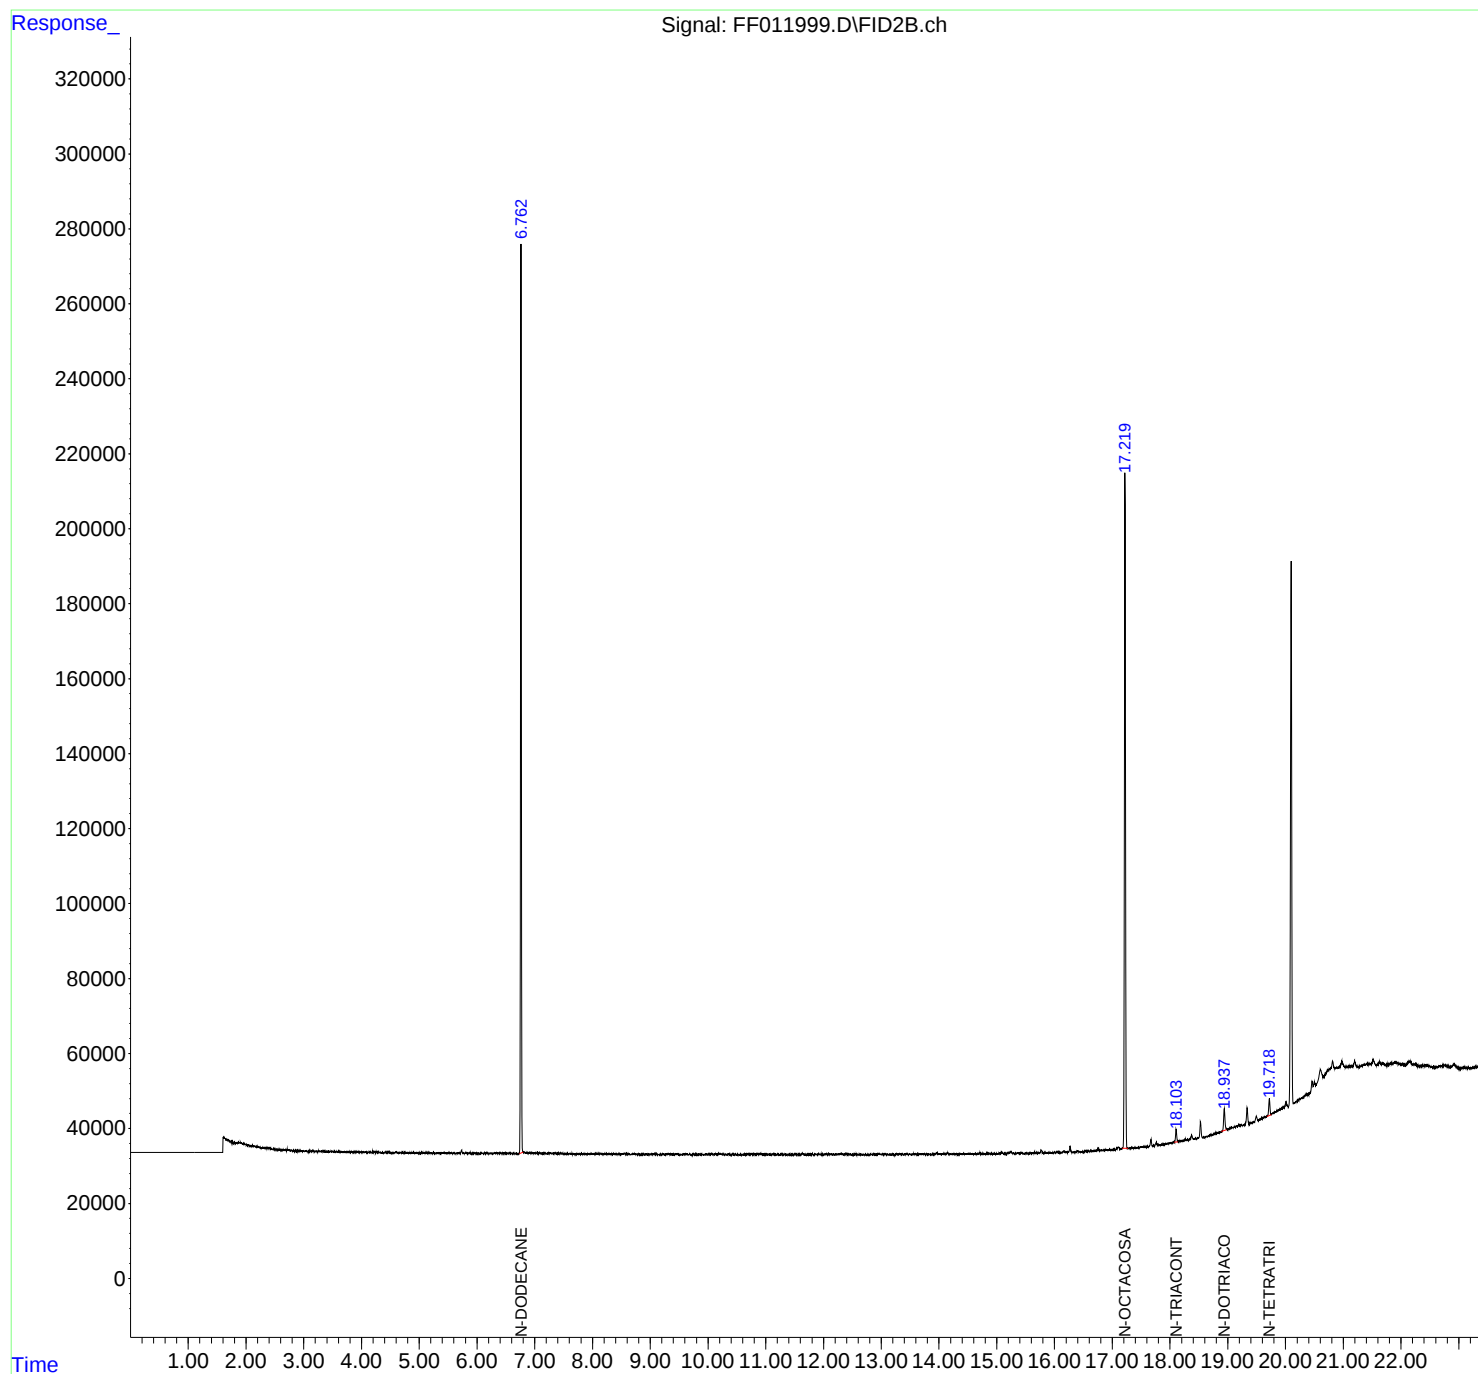


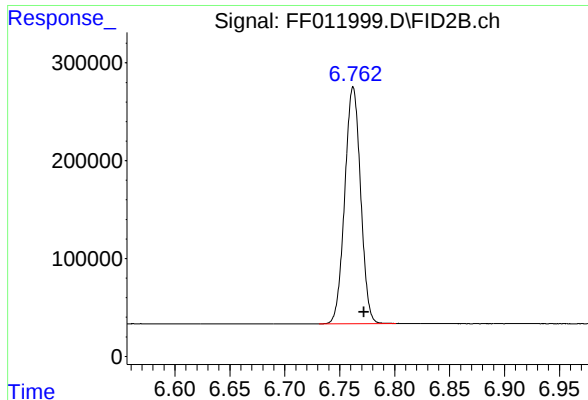

#3 N-DODECANE


R.T.: 6.762 min
Delta R.T.: -0.010 min
Response: 2428706
Conc: 20.27 ug/ml

Instrument :
FID_F
ClientSampleId :

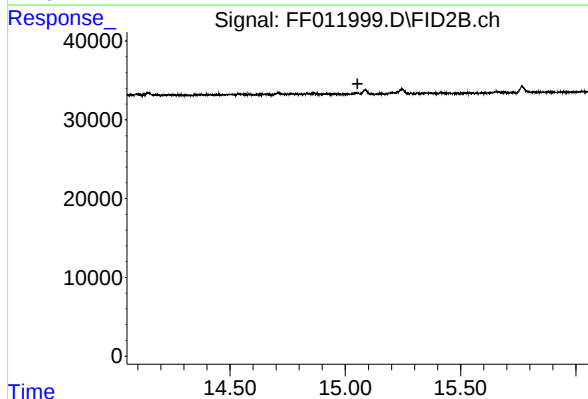


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

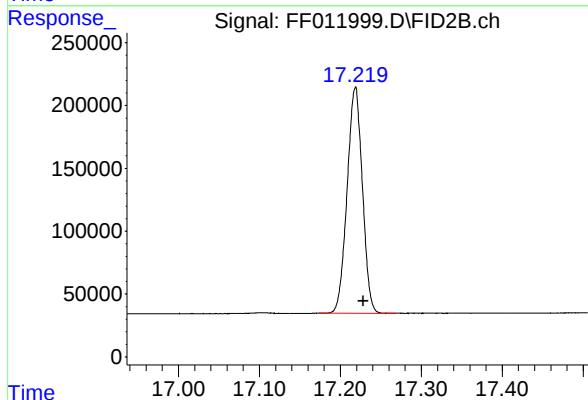


#12 N-OCTACOSANE

R.T.: 17.219 min
Delta R.T.: -0.010 min
Response: 2360662
Conc: 18.15 ug/ml

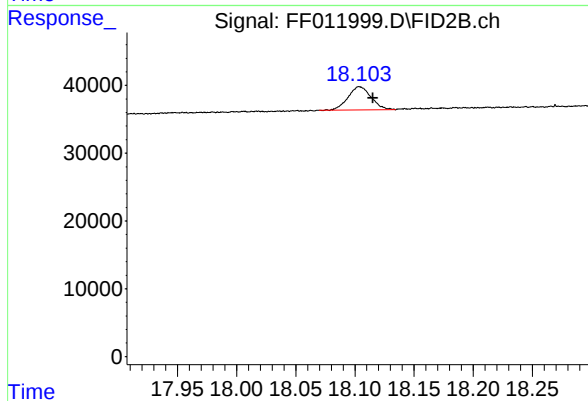

#13 N-TRIACONTANE


R.T.: 18.104 min
Delta R.T.: -0.011 min
Response: 47058
Conc: 0.36 ug/ml

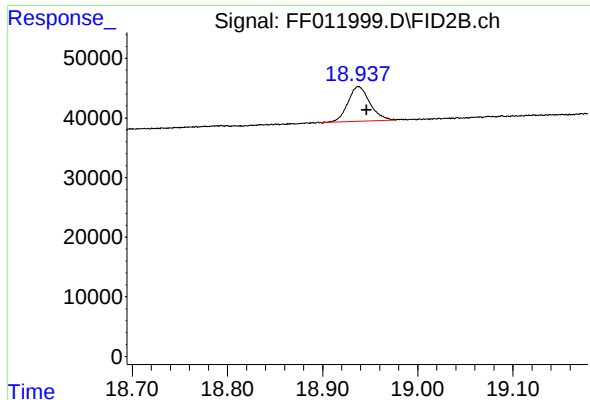

#14 N-DOTRIACONTANE

R.T.: 18.938 min
Delta R.T.: -0.009 min
Response: 93810
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

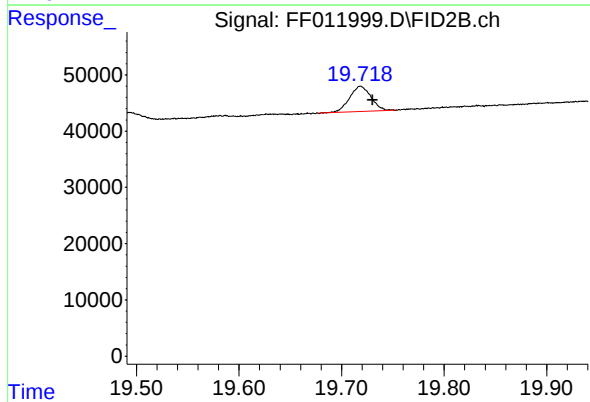

#15 N-TETRATRIACONTANE

R.T.: 19.719 min
Delta R.T.: -0.012 min
Response: 65700
Conc: 0.59 ug/ml