

Data Path : P:\HPCHEM1\FID_F\Data\FF020818\
 Data File : FF000073.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2018 12:18
 Operator : UA\AJ
 Sample : WATER MDL 07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 08 13:18:18 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
 Quant Title :
 QLast Update : Fri Feb 02 10:05:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	2280975	20.027 ug/ml
Target Compounds			
1) N-OCTANE	2.294	145696	0.962 ug/ml
2) N-DECANE	4.384	162237	1.048 ug/ml
3) N-DODECANE	6.399	163895	1.061 ug/ml
4) N-TETRADECANE	8.189	163747	1.072 ug/ml
5) N-HEXADECANE	9.787	161887	1.101 ug/ml
6) N-OCTADECANE	11.227	155816	1.071 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF020818\
Data File : FF000073.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2018 12:18
Operator : UA\AJ
Sample : WATER MDL 07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 13:18:18 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
Quant Title :
QLast Update : Fri Feb 02 10:05:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

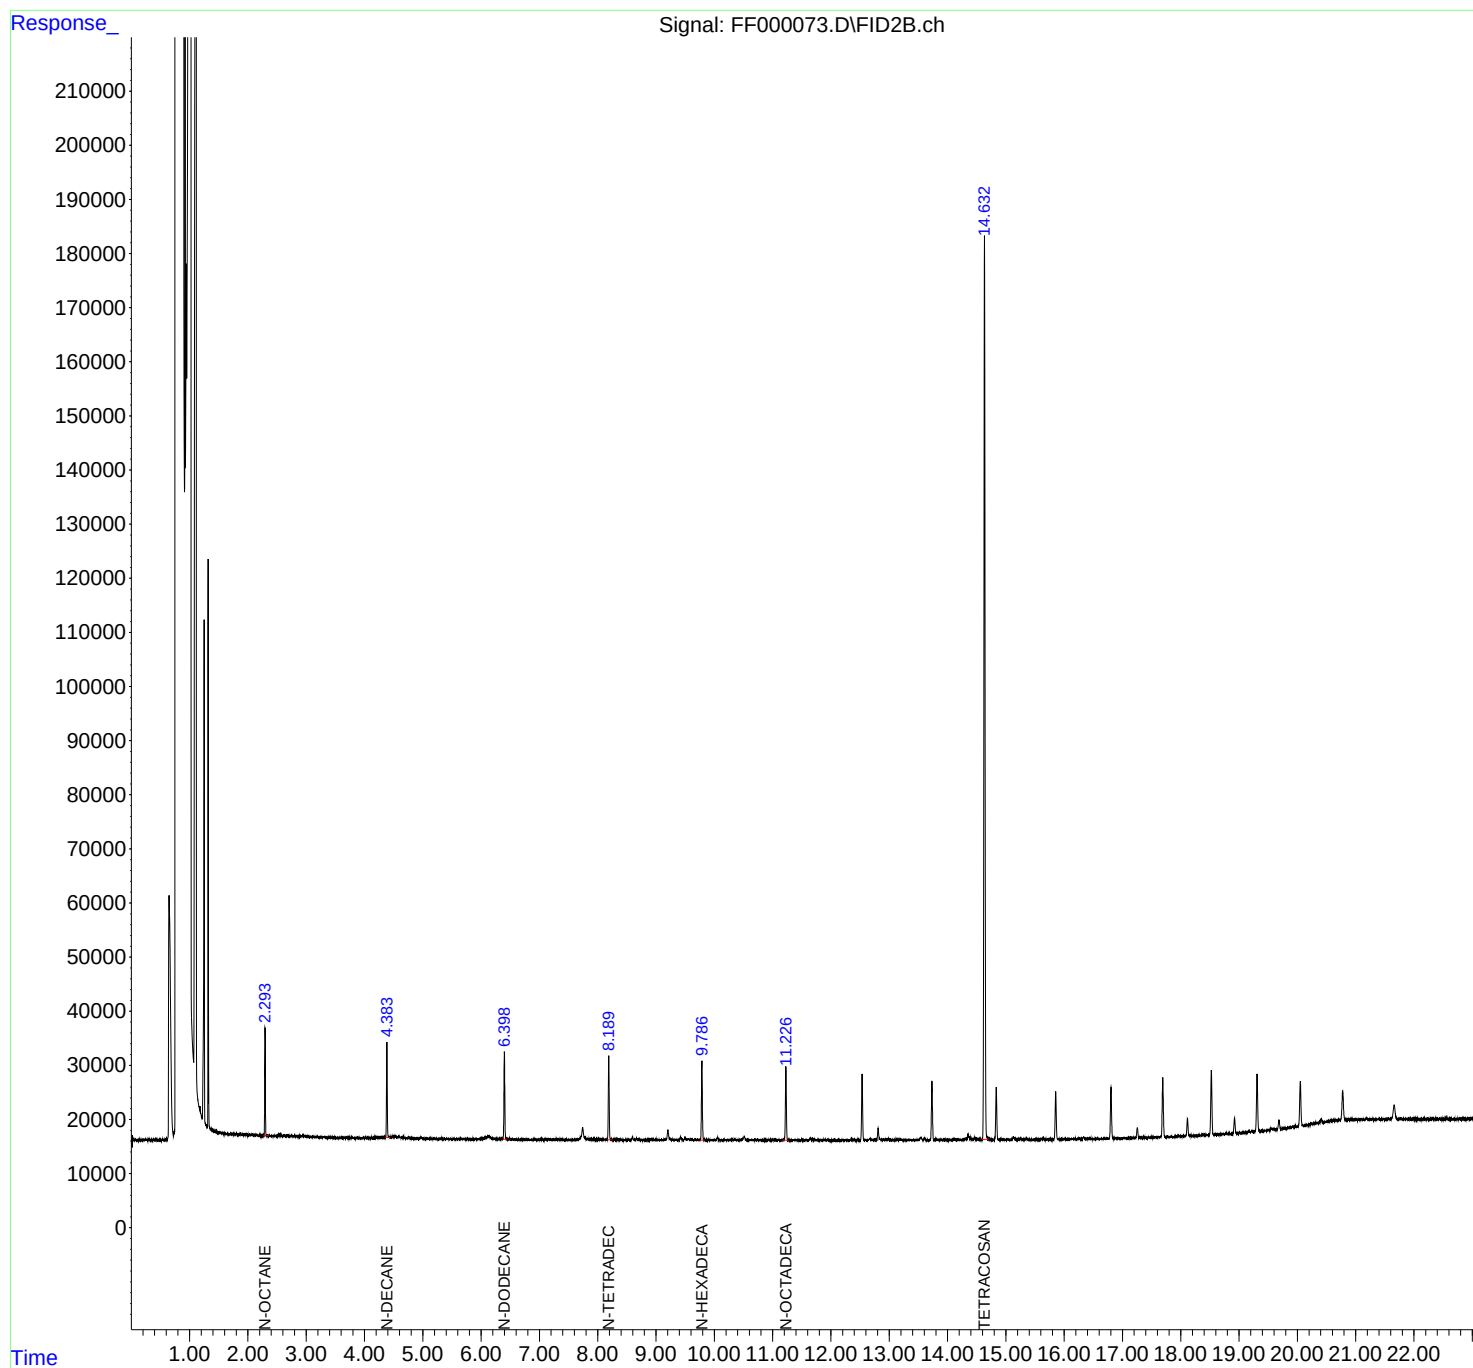

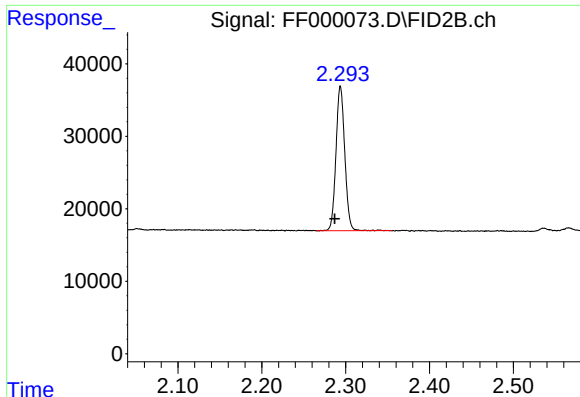


#1 N-OCTANE

R.T.: 2.294 min
Delta R.T.: 0.007 min
Response: 145696
Conc: 0.96 ug/ml

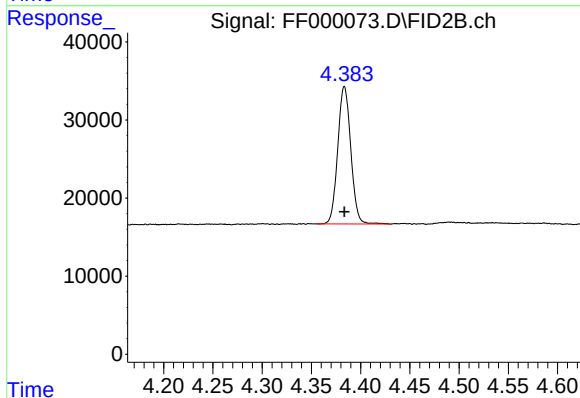


#2 N-DECANE

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 162237
Conc: 1.05 ug/ml

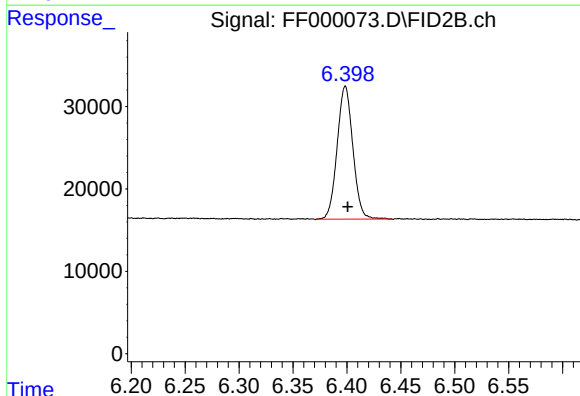


#3 N-DODECANE

R.T.: 6.399 min
Delta R.T.: -0.002 min
Response: 163895
Conc: 1.06 ug/ml

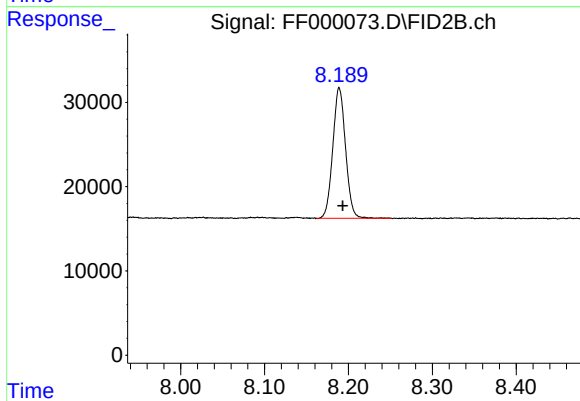


#4 N-TETRADECANE

R.T.: 8.189 min
Delta R.T.: -0.004 min
Response: 163747
Conc: 1.07 ug/ml

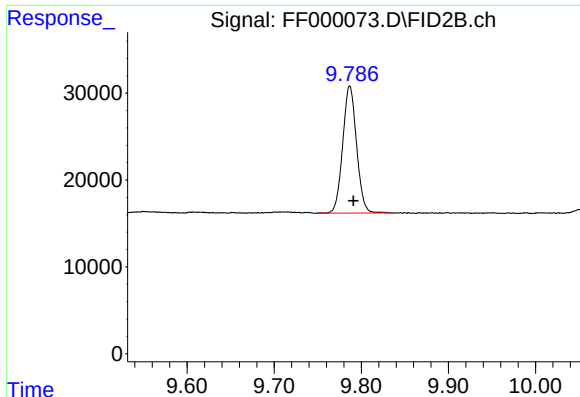


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: -0.004 min
Response: 161887
Conc: 1.10 ug/ml

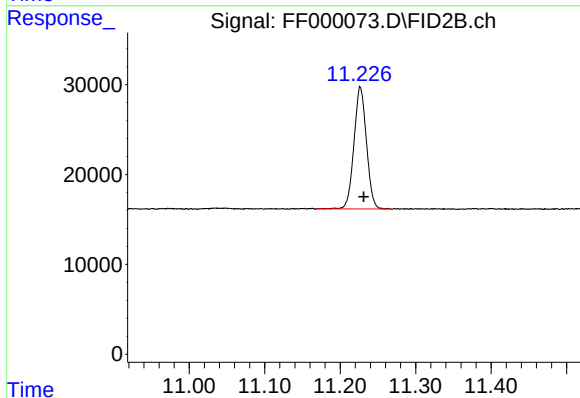

#6 N-OCTADECANE

R.T.: 11.227 min
Delta R.T.: -0.004 min
Response: 155816
Conc: 1.07 ug/ml

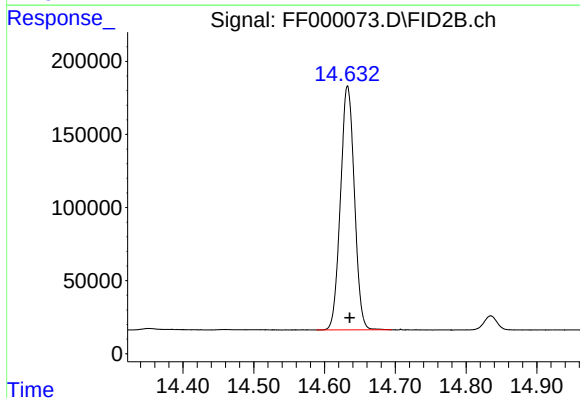

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: -0.003 min
Response: 2280975
Conc: 20.03 ug/ml