

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020819\
 Data File : FF003443.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2019 18:43
 Operator : AJ\SJ
 Sample : K1385-01 2X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 08 21:51:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	1082479	8.966 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213f	220025	1.626 ug/ml
5) N-HEXADECANE	9.758	100724	0.739 ug/ml
7) N-EICOSANE	12.513	140320	1.020 ug/ml
8) N-DOCOSANE	13.732	292664	2.139 ug/ml
10) N-TETRACOSANE	14.791	1395180	10.259 ug/ml
11) N-HEXACOSANE	15.847	203674	1.502 ug/ml
12) N-OCTACOSANE	16.799	683381	4.991 ug/ml
13) N-TRIACONTANE	17.691	560998	3.973 ug/ml
14) N-DOTRIACONTANE	18.524	434210	3.146 ug/ml
15) N-TETRATRIACONTANE	19.314	110600	0.872 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020819\
Data File : FF003443.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2019 18:43
Operator : AJ\SJ
Sample : K1385-01 2X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 21:51:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

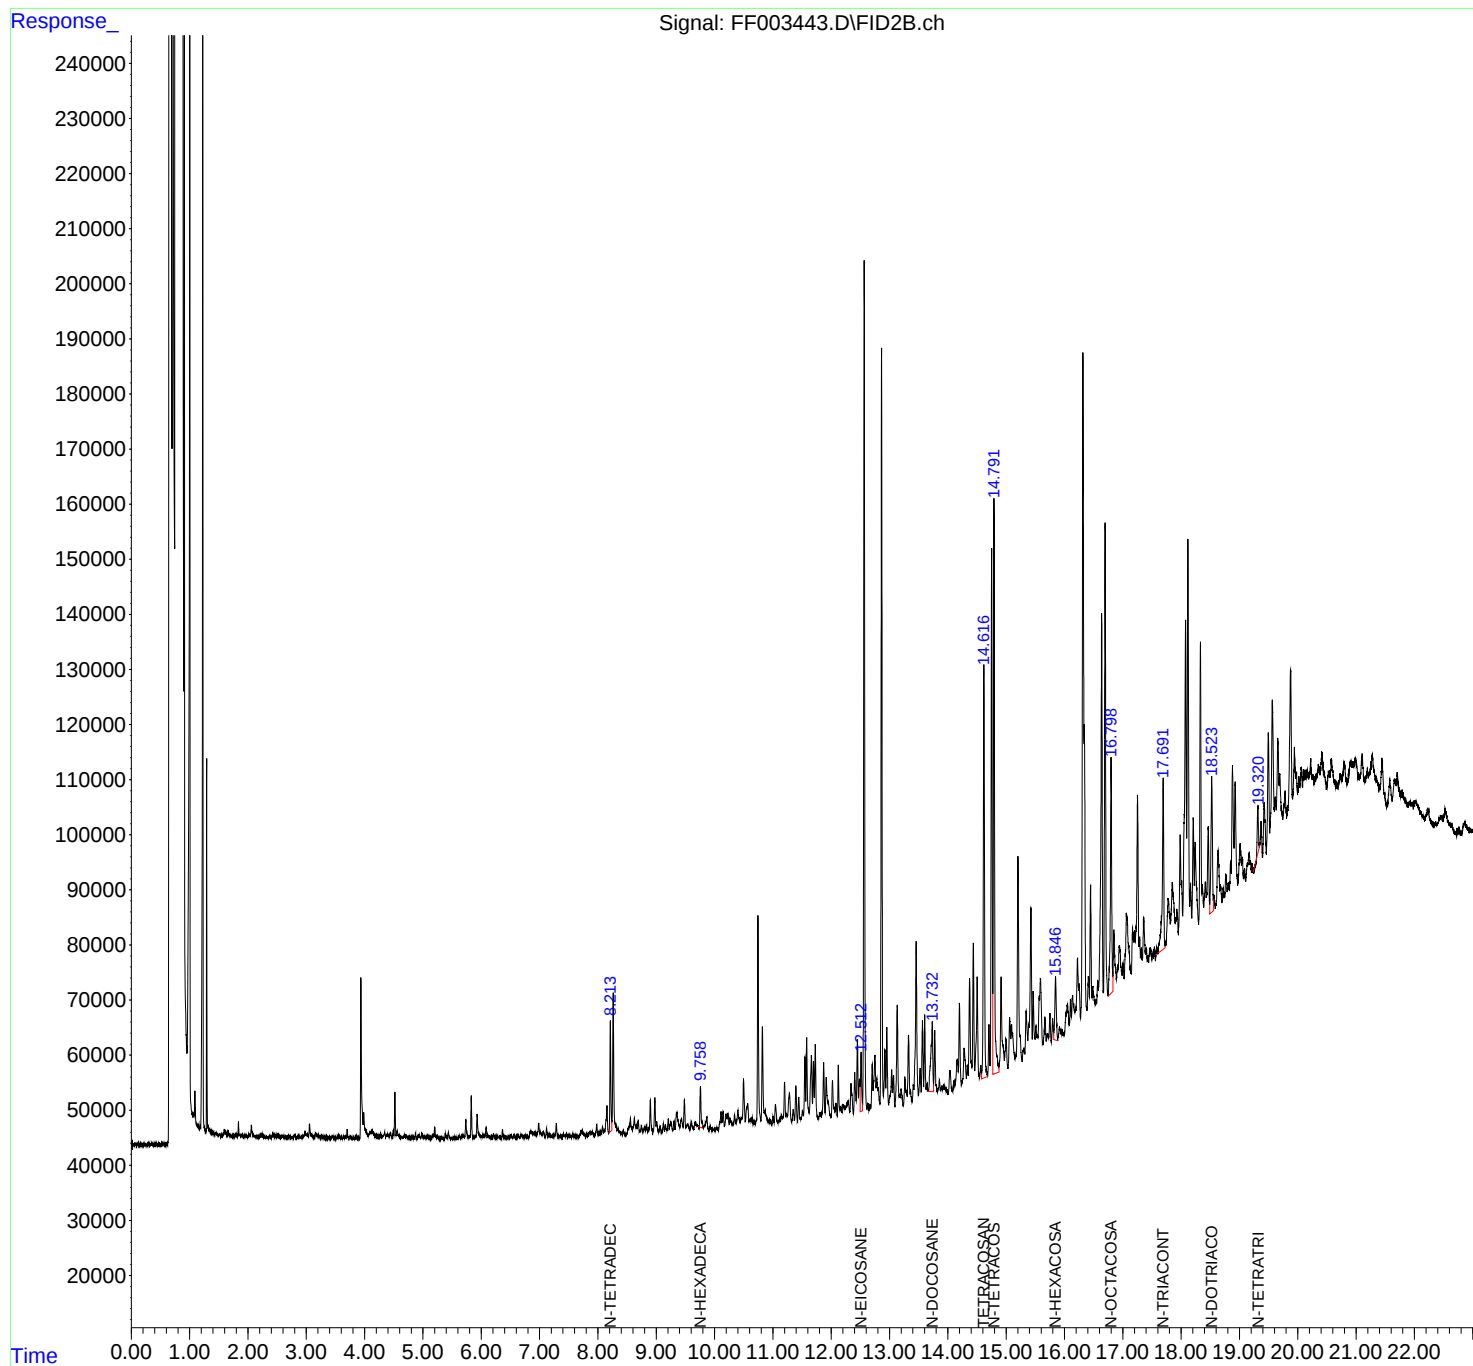

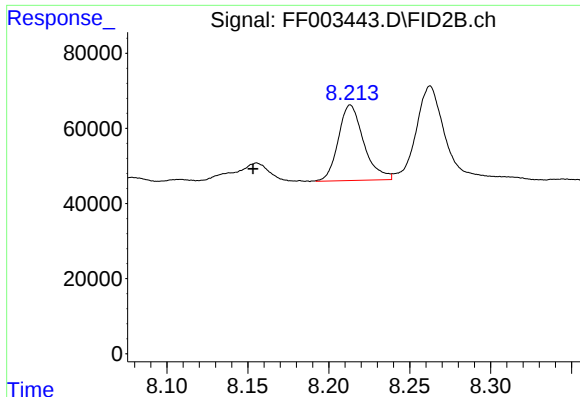


#4 N-TETRADECANE

R.T.: 8.213 min
Delta R.T.: 0.060 min
Response: 220025
Conc: 1.63 ug/ml

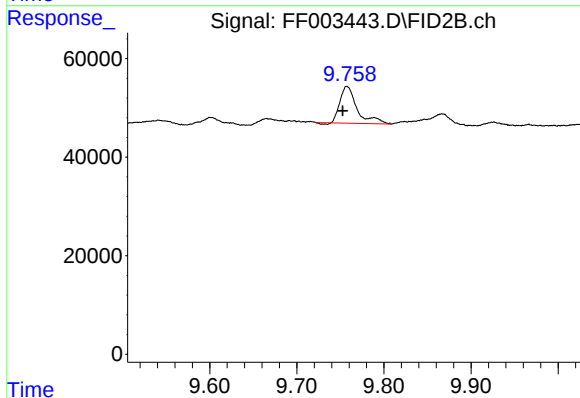


#5 N-HEXADECANE

R.T.: 9.758 min
Delta R.T.: 0.005 min
Response: 100724
Conc: 0.74 ug/ml

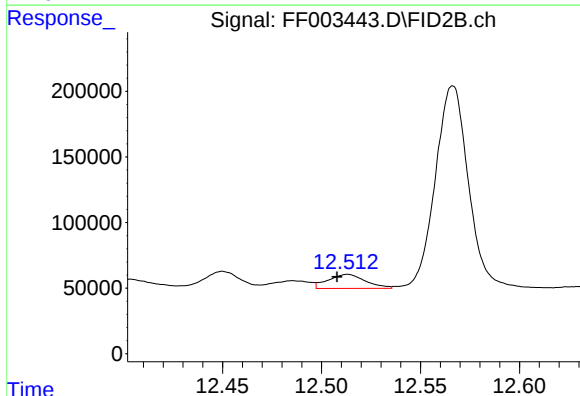


#7 N-EICOSANE

R.T.: 12.513 min
Delta R.T.: 0.005 min
Response: 140320
Conc: 1.02 ug/ml

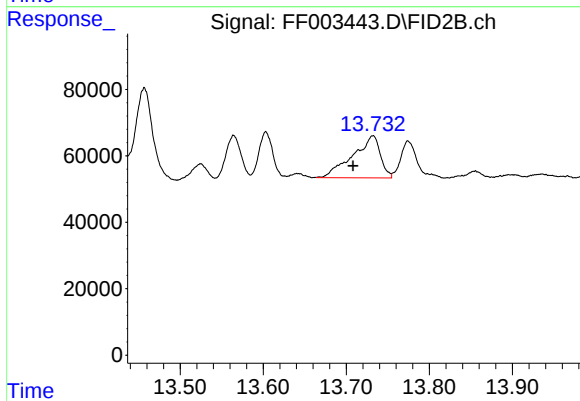


#8 N-DOCOSANE

R.T.: 13.732 min
Delta R.T.: 0.024 min
Response: 292664
Conc: 2.14 ug/ml

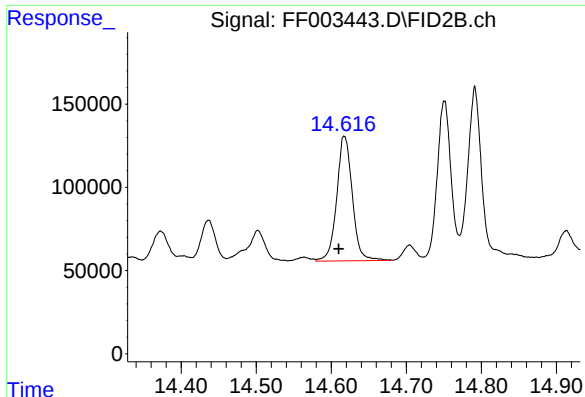


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min
Delta R.T.: 0.007 min
Response: 1082479
Conc: 8.97 ug/ml

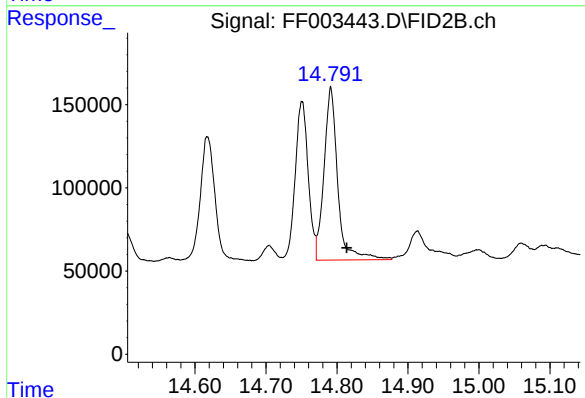


#10 N-TETRACOSANE

R.T.: 14.791 min
Delta R.T.: -0.022 min
Response: 1395180
Conc: 10.26 ug/ml

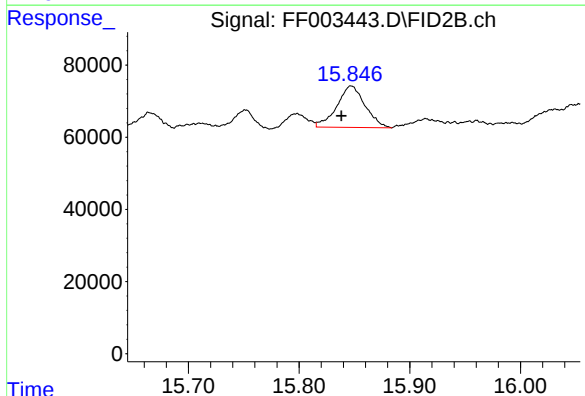


#11 N-HEXACOSANE

R.T.: 15.847 min
Delta R.T.: 0.009 min
Response: 203674
Conc: 1.50 ug/ml

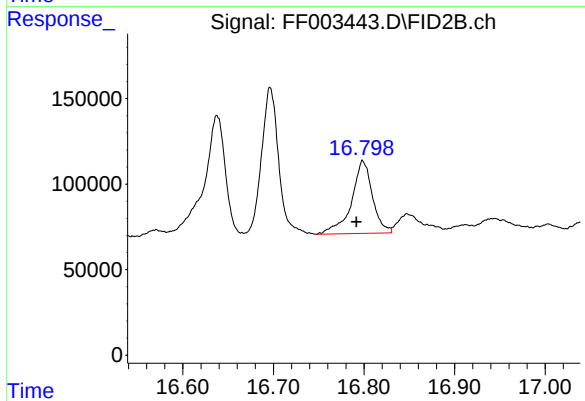


#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: 0.007 min
Response: 683381
Conc: 4.99 ug/ml

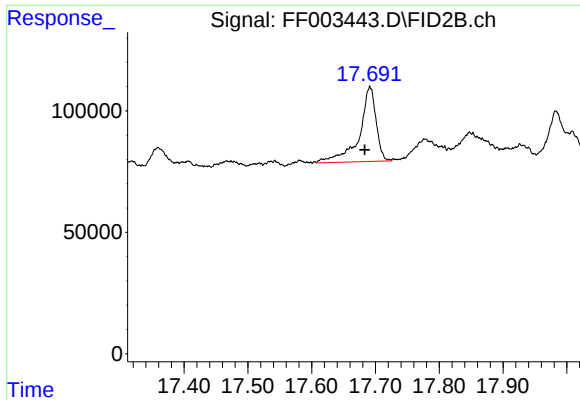


#13 N-TRIACONTANE

R.T.: 17.691 min
Delta R.T.: 0.008 min
Response: 560998
Conc: 3.97 ug/ml

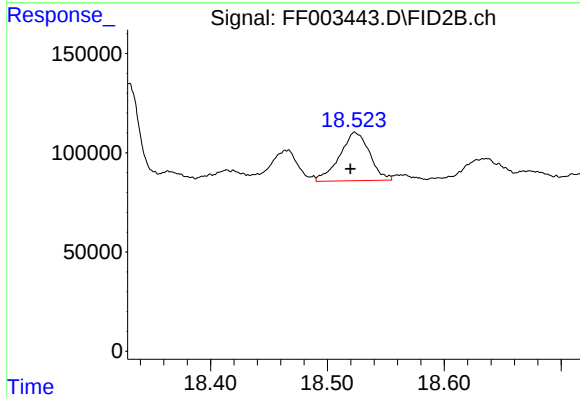

#14 N-DOTRIACONTANE

R.T.: 18.524 min
Delta R.T.: 0.004 min
Response: 434210
Conc: 3.15 ug/ml

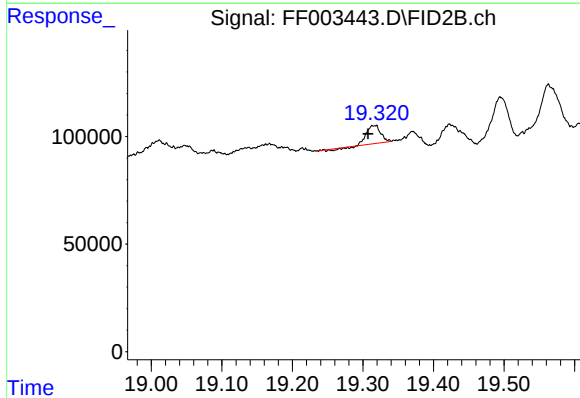

#15 N-TETRATRIACONTANE

R.T.: 19.314 min
Delta R.T.: 0.007 min
Response: 110600
Conc: 0.87 ug/ml