

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
Data File : FF009914.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2022 09:34
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 21:30:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.084	264814	2.230 ug/ml
16) N-HEXATRIACONTANE	19.866	895101	8.682 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
Data File : FF009914.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2022 09:34
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 21:30:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

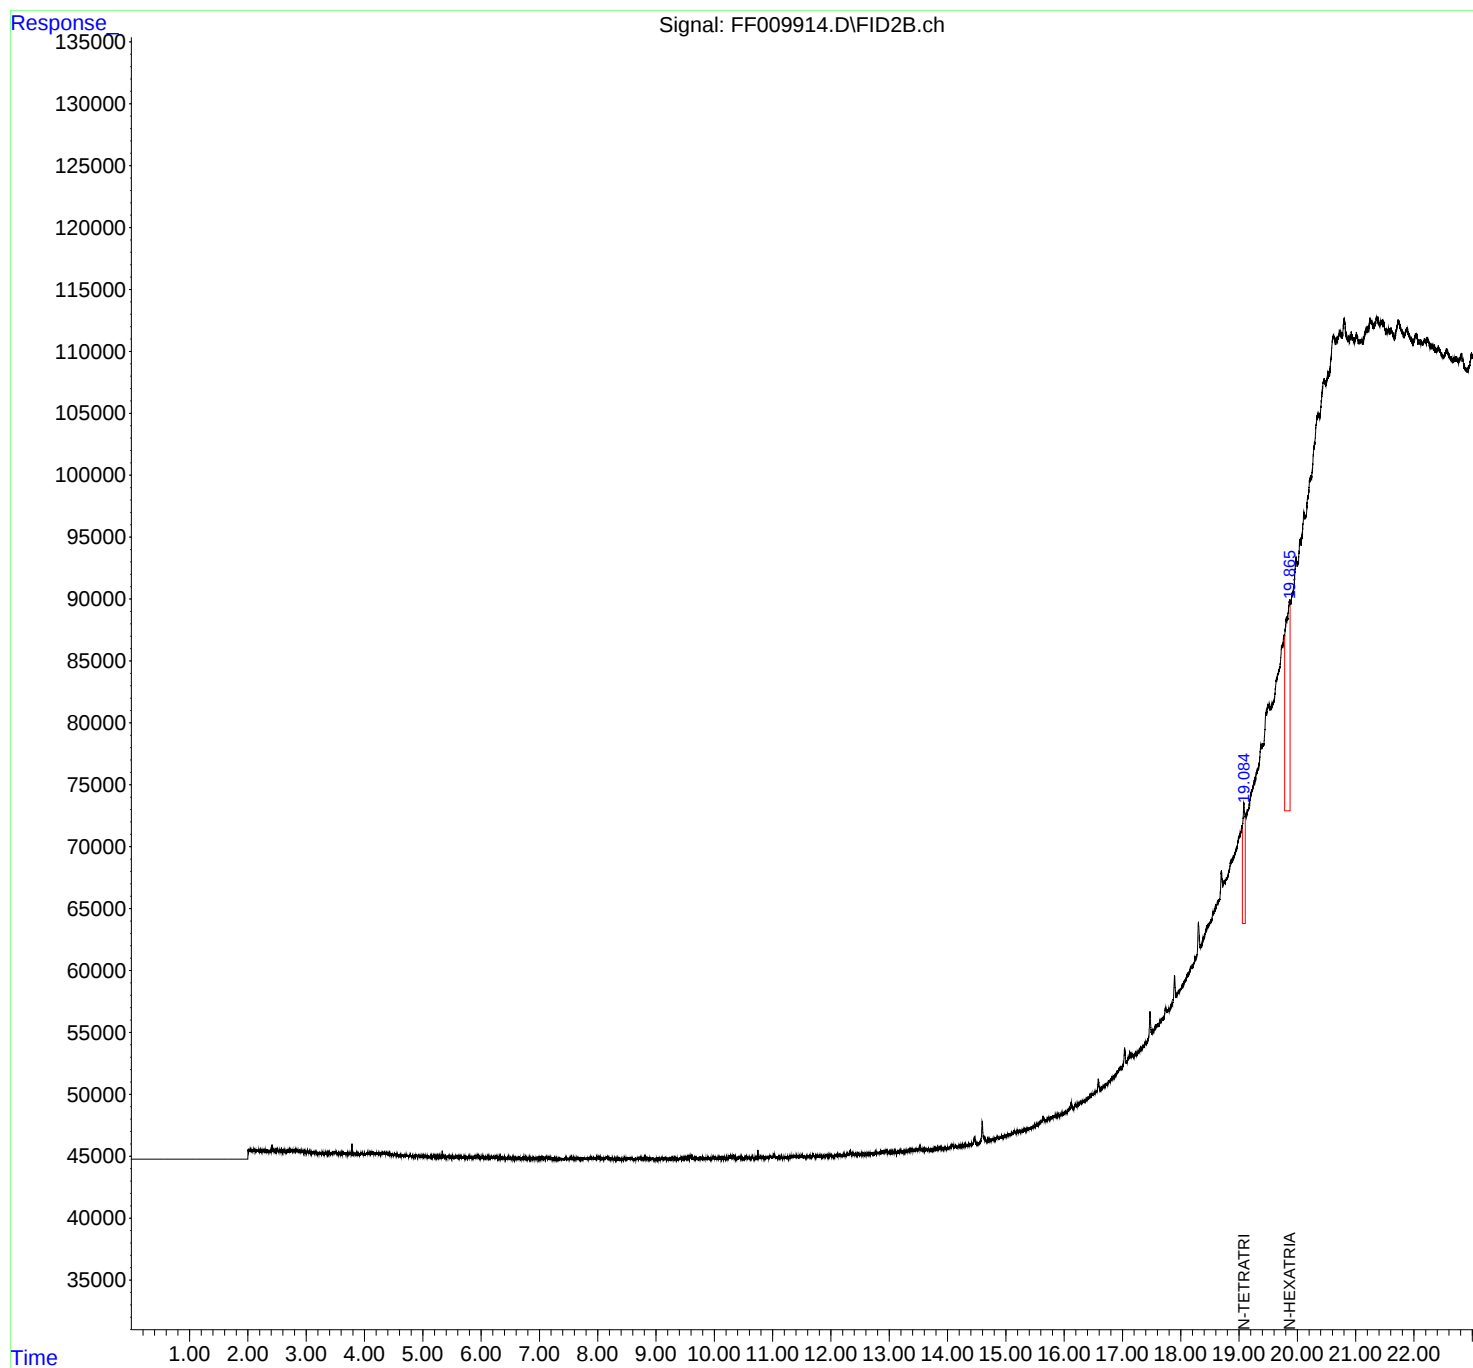


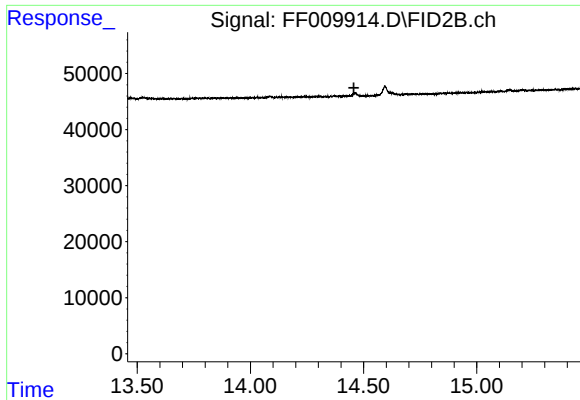

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

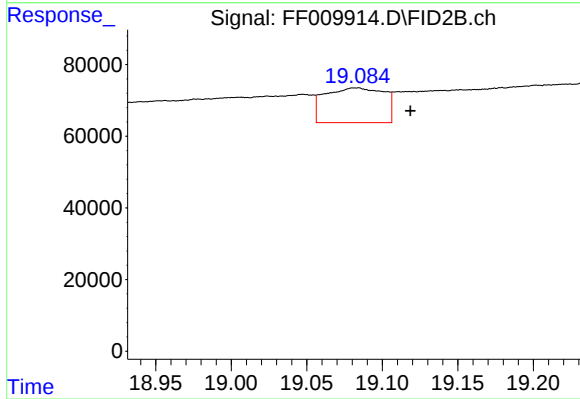

#15 N-TETRATRIACONTANE

R.T.: 19.084 min
Delta R.T.: -0.034 min
Response: 264814
Conc: 2.23 ug/ml

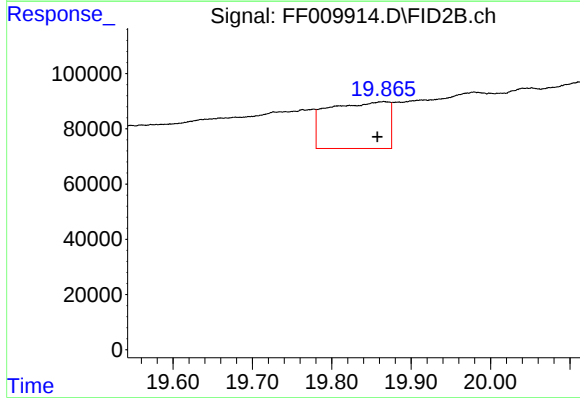

#16 N-HEXATRIACONTANE

R.T.: 19.866 min
Delta R.T.: 0.008 min
Response: 895101
Conc: 8.68 ug/ml