

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
 Data File : FF009918.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2022 12:07
 Operator : AJ\MA
 Sample : N1422-01 20X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 08 21:31:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.422	184786	1.414 ug/ml
Target Compounds			
3) N-DODECANE	6.259	4403	0.031 ug/ml
7) N-EICOSANE	12.406	34039	0.225 ug/ml
10) N-TETRACOSANE	14.642	354135	2.388 ug/ml
11) N-HEXACOSANE	15.637	64441	0.441 ug/ml
12) N-OCTACOSANE	16.588	255906	1.763 ug/ml
13) N-TRIACONTANE	17.467	365158	2.552 ug/ml
14) N-DOTRIACONTANE	18.303	143332	1.053 ug/ml
15) N-TETRATRIACONTANE	19.097	175072	1.474 ug/ml
16) N-HEXATRIACONTANE	19.871	266101	2.581 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
Data File : FF009918.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2022 12:07
Operator : AJ\MA
Sample : N1422-01 20X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 21:31:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

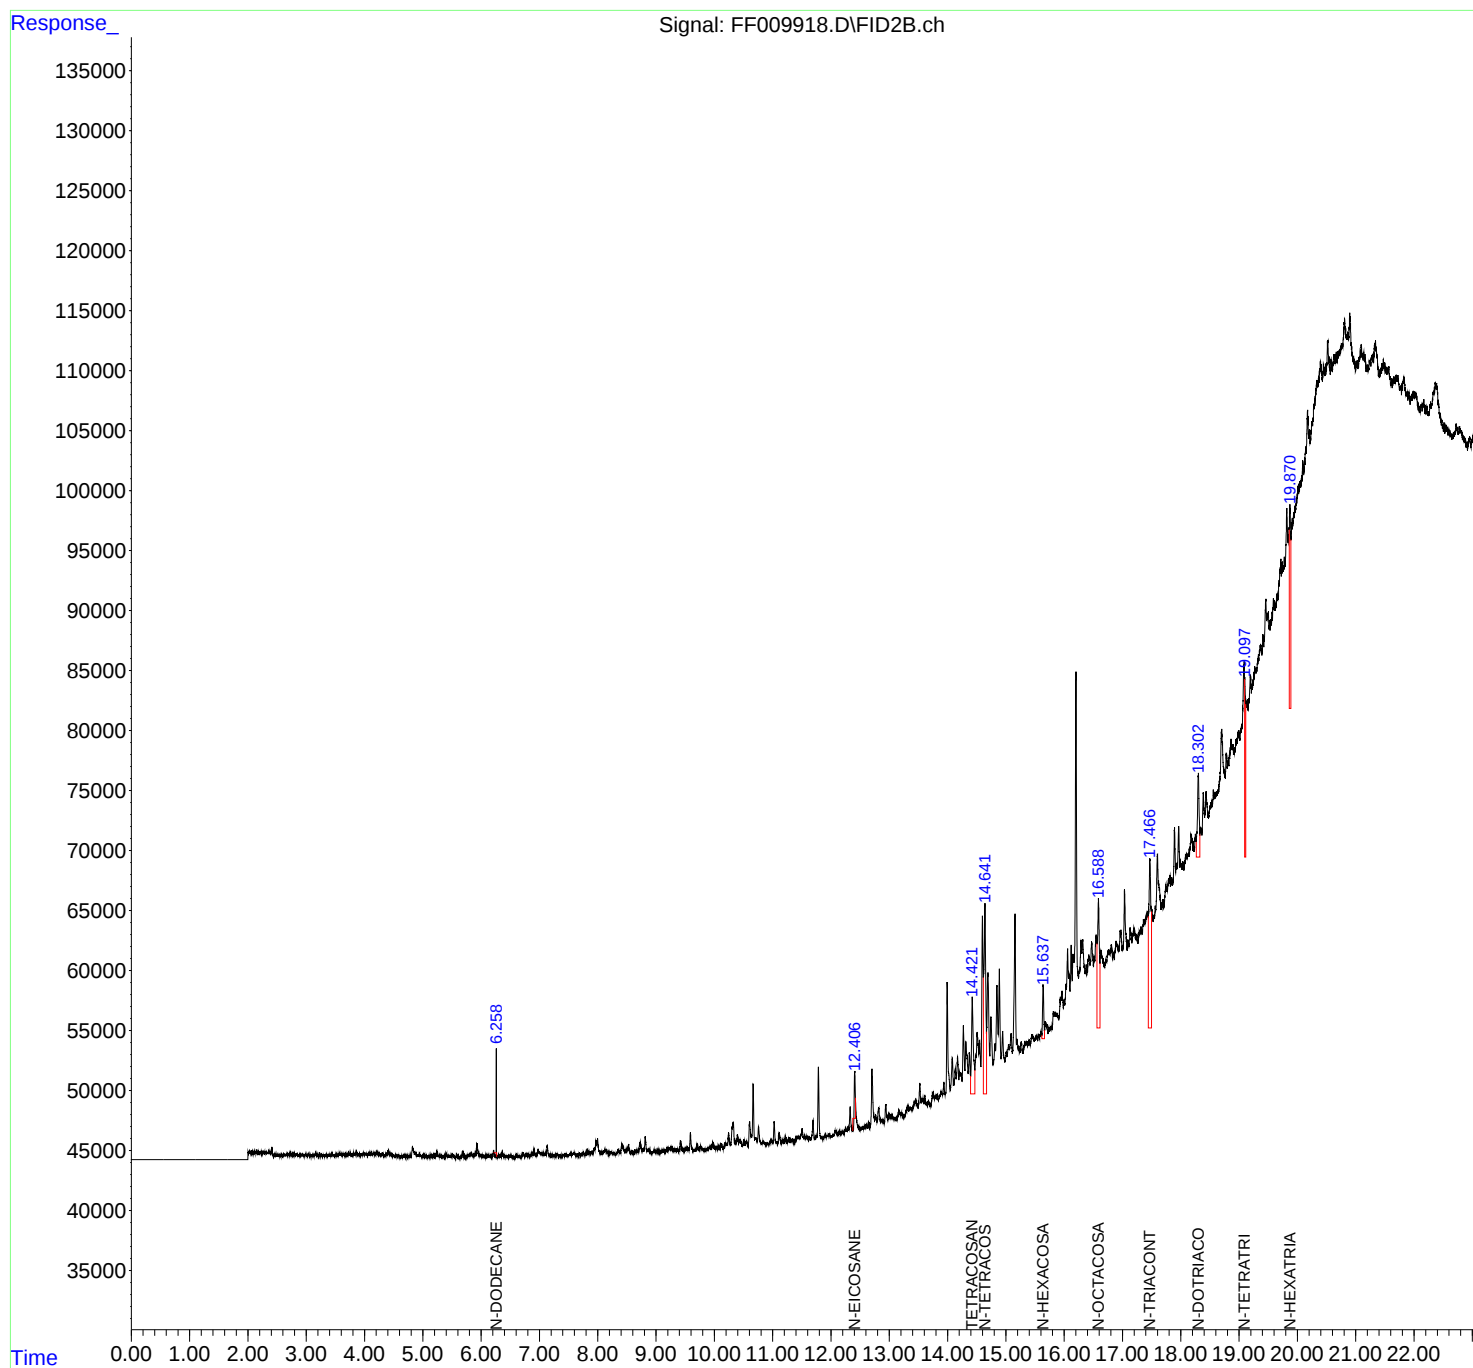


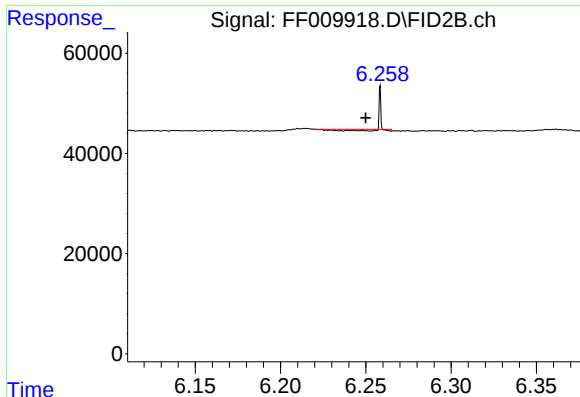

#3 N-DODECANE


R.T.: 6.259 min
Delta R.T.: 0.009 min
Response: 4403
Conc: 0.03 ug/ml

Instrument :
FID_F
ClientSampleId :

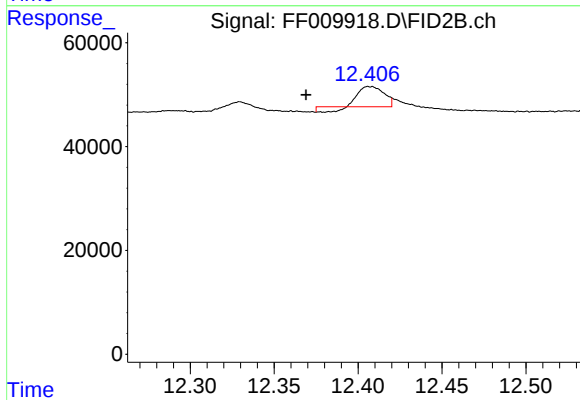


#7 N-EICOSANE

R.T.: 12.406 min
Delta R.T.: 0.037 min
Response: 34039
Conc: 0.23 ug/ml

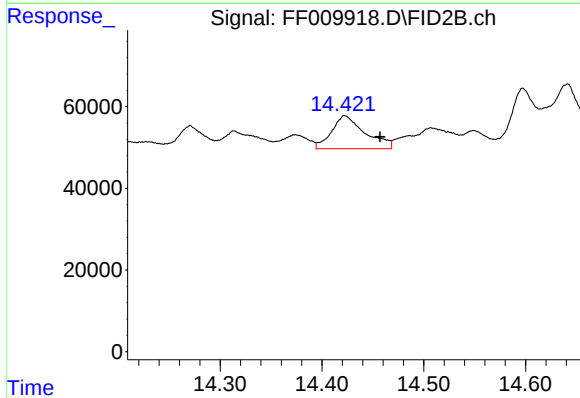


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.422 min
Delta R.T.: -0.035 min
Response: 184786
Conc: 1.41 ug/ml

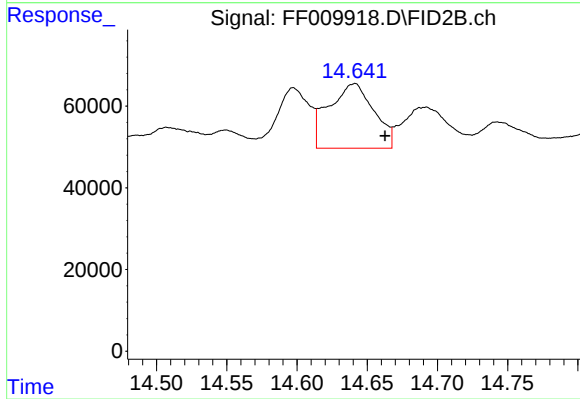

#10 N-TETRACOSANE


R.T.: 14.642 min
Delta R.T.: -0.021 min
Response: 354135
Conc: 2.39 ug/ml

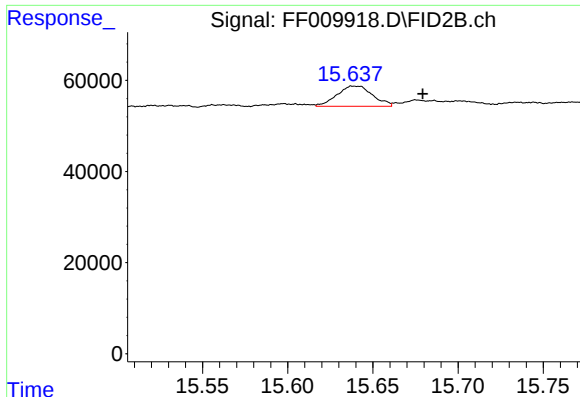

#11 N-HEXACOSANE


R.T.: 15.637 min
Delta R.T.: -0.042 min
Response: 64441
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

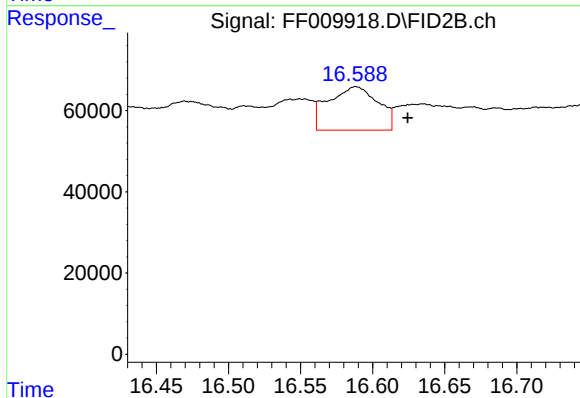


#12 N-OCTACOSANE

R.T.: 16.588 min
Delta R.T.: -0.036 min
Response: 255906
Conc: 1.76 ug/ml

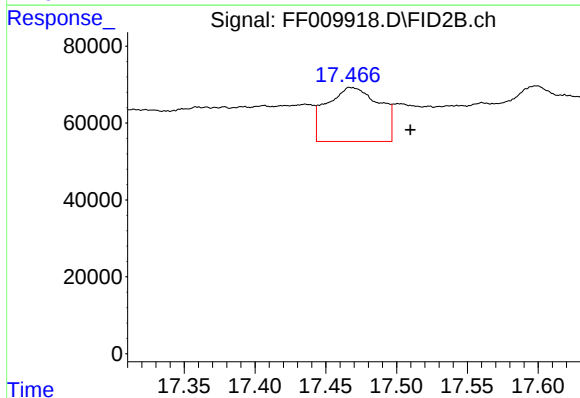


#13 N-TRIACONTANE

R.T.: 17.467 min
Delta R.T.: -0.043 min
Response: 365158
Conc: 2.55 ug/ml

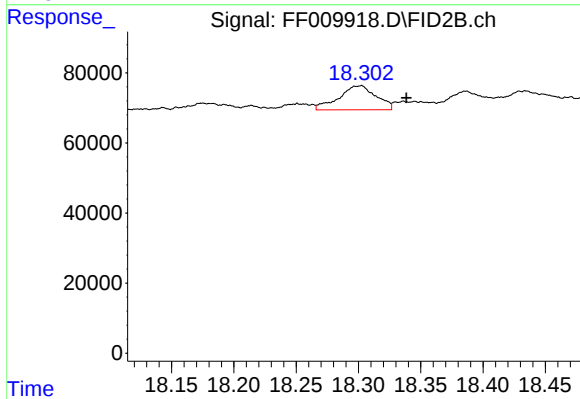

#14 N-DOTRIACONTANE


R.T.: 18.303 min
Delta R.T.: -0.036 min
Response: 143332
Conc: 1.05 ug/ml

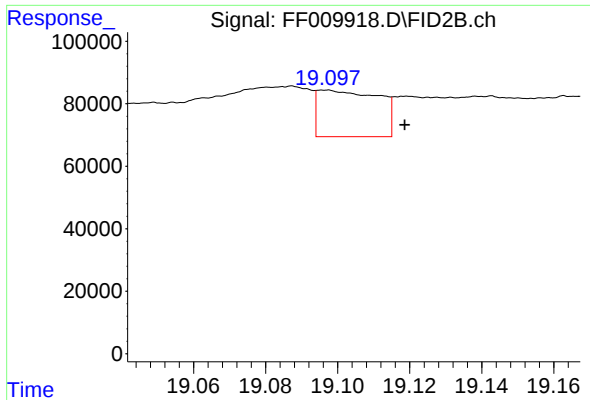

#15 N-TETRATRIACONTANE

R.T.: 19.097 min
Delta R.T.: -0.021 min
Response: 175072
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :

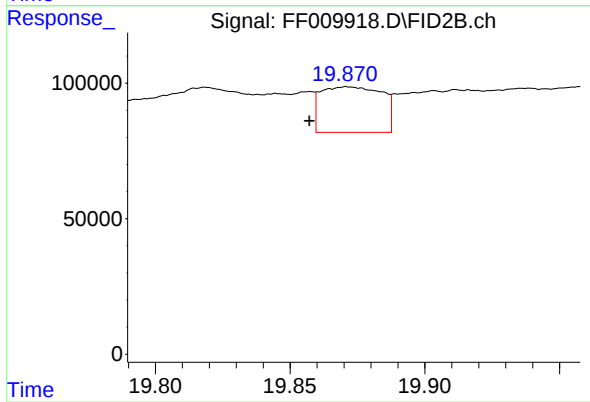

#16 N-HEXATRIACONTANE

R.T.: 19.871 min
Delta R.T.: 0.014 min
Response: 266101
Conc: 2.58 ug/ml