

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
Data File : FG0TEST.D
Signal(s) : FID1A.ch
Acq On : 08 Feb 2022 14:15
Operator : AJ\MA
Sample : test
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 21:32:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.720f	7006291	47.244 ug/ml
14)	N-DOTRIACONTANE	18.272f	85776	0.630 ug/ml
15)	N-TETRATRIACONTANE	19.096	138383	1.165 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020822\
Data File : FG0TEST.D
Signal(s) : FID1A.ch
Acq On : 08 Feb 2022 14:15
Operator : AJ\MA
Sample : test
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 21:32:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

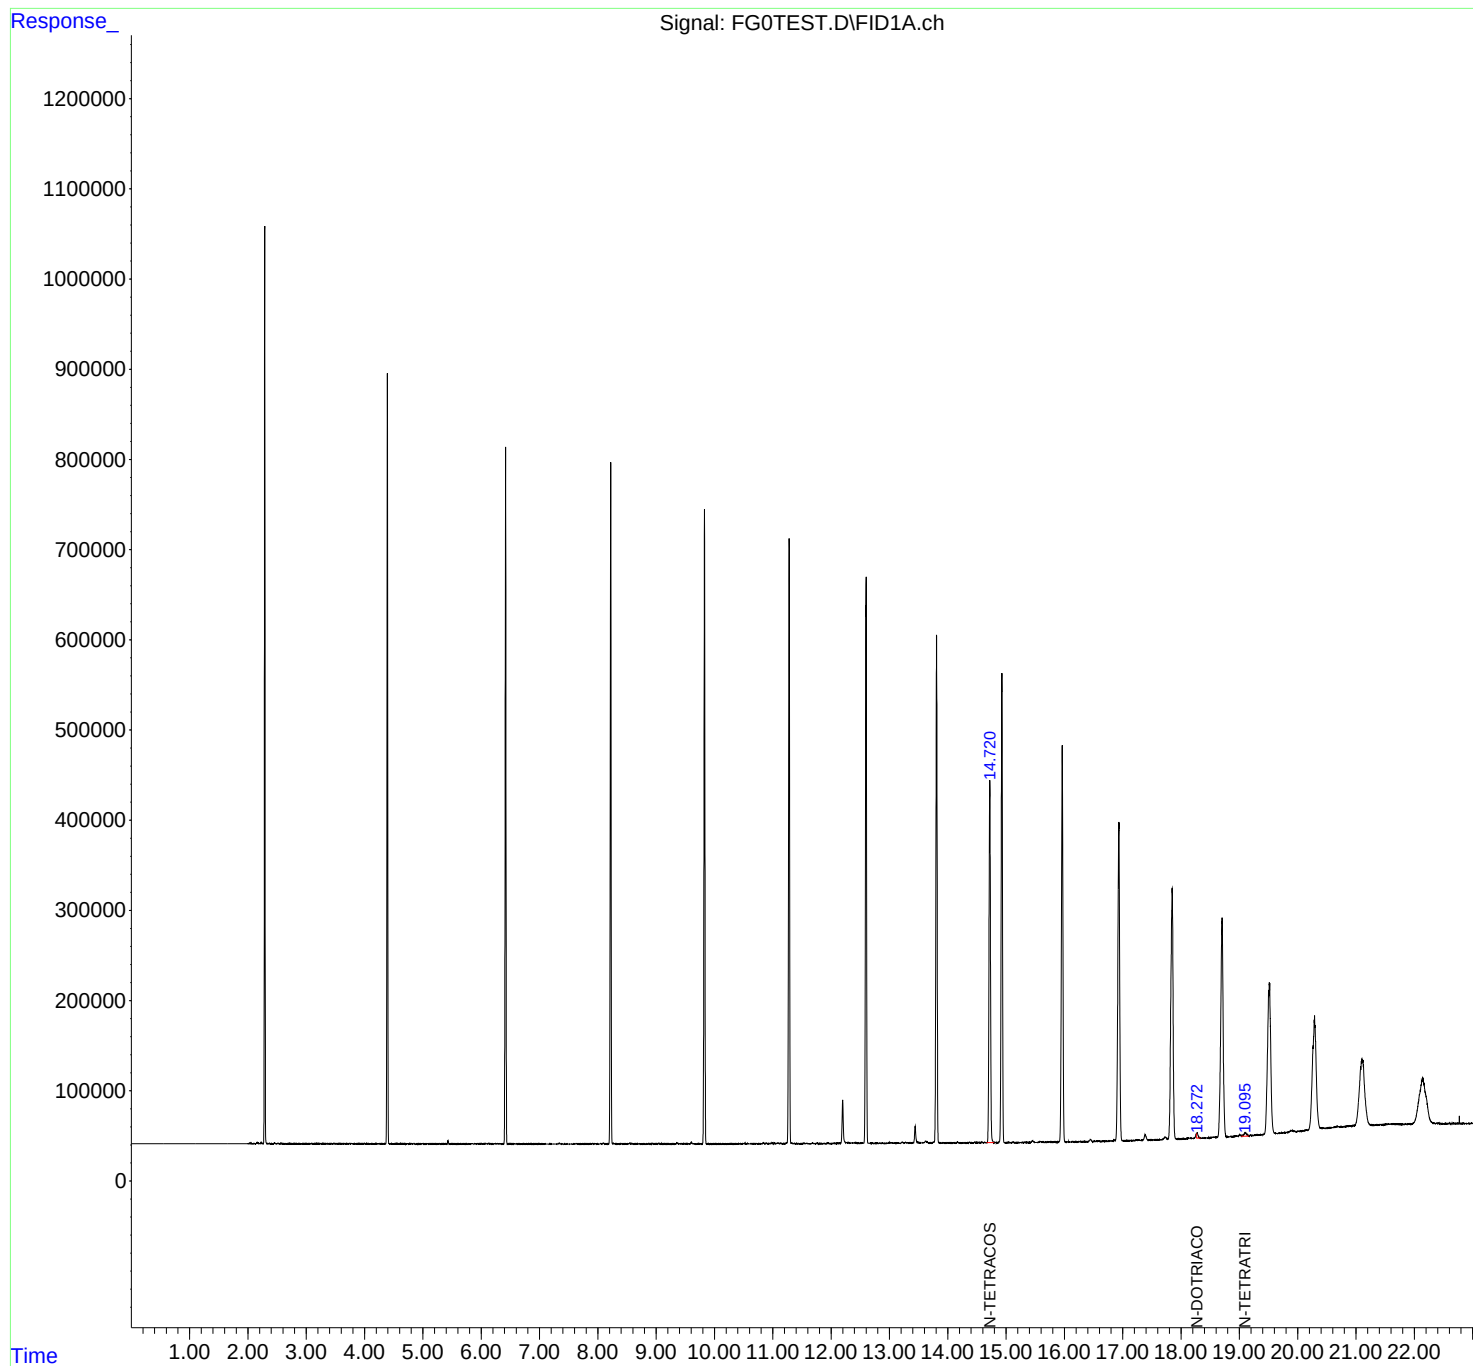


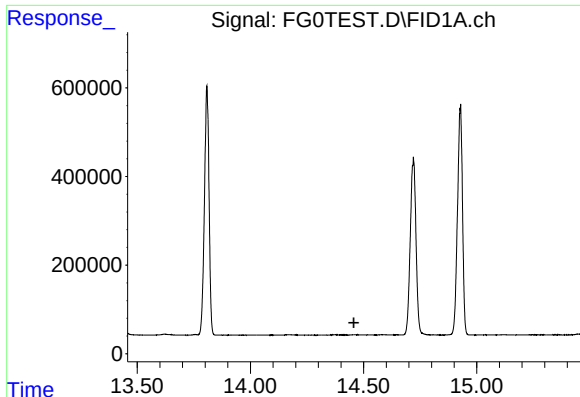

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

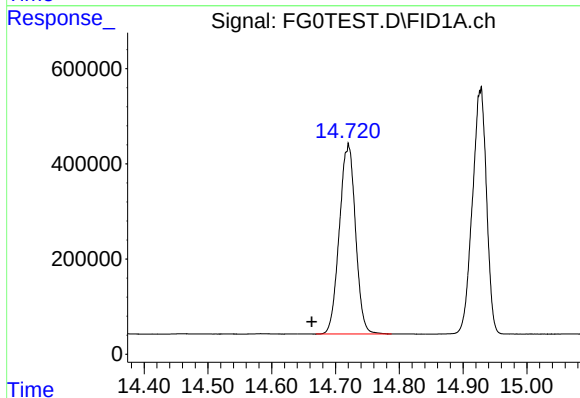


#10 N-TETRACOSANE

R.T.: 14.720 min
Delta R.T.: 0.058 min
Response: 7006291
Conc: 47.24 ug/ml

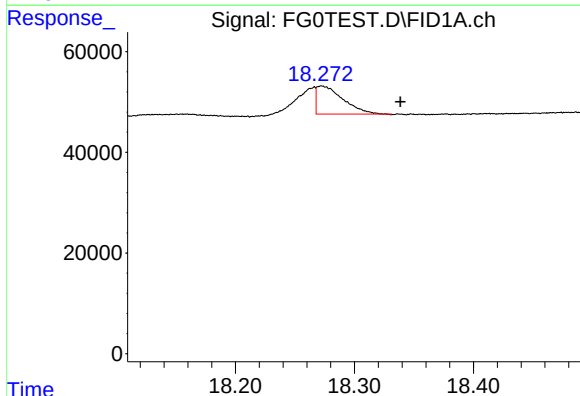

#14 N-DOTRIACONTANE

R.T.: 18.272 min
Delta R.T.: -0.066 min
Response: 85776
Conc: 0.63 ug/ml

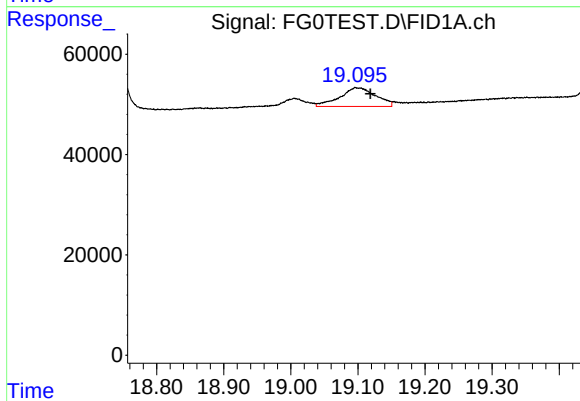

#15 N-TETRATRIACONTANE

R.T.: 19.096 min
Delta R.T.: -0.022 min
Response: 138383
Conc: 1.17 ug/ml