

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012003.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 10:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 09 02:43:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.936	66111	0.508 ug/ml
15) N-TETRATRIACONTANE	19.719	48899	0.439 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012003.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 10:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 09 02:43:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

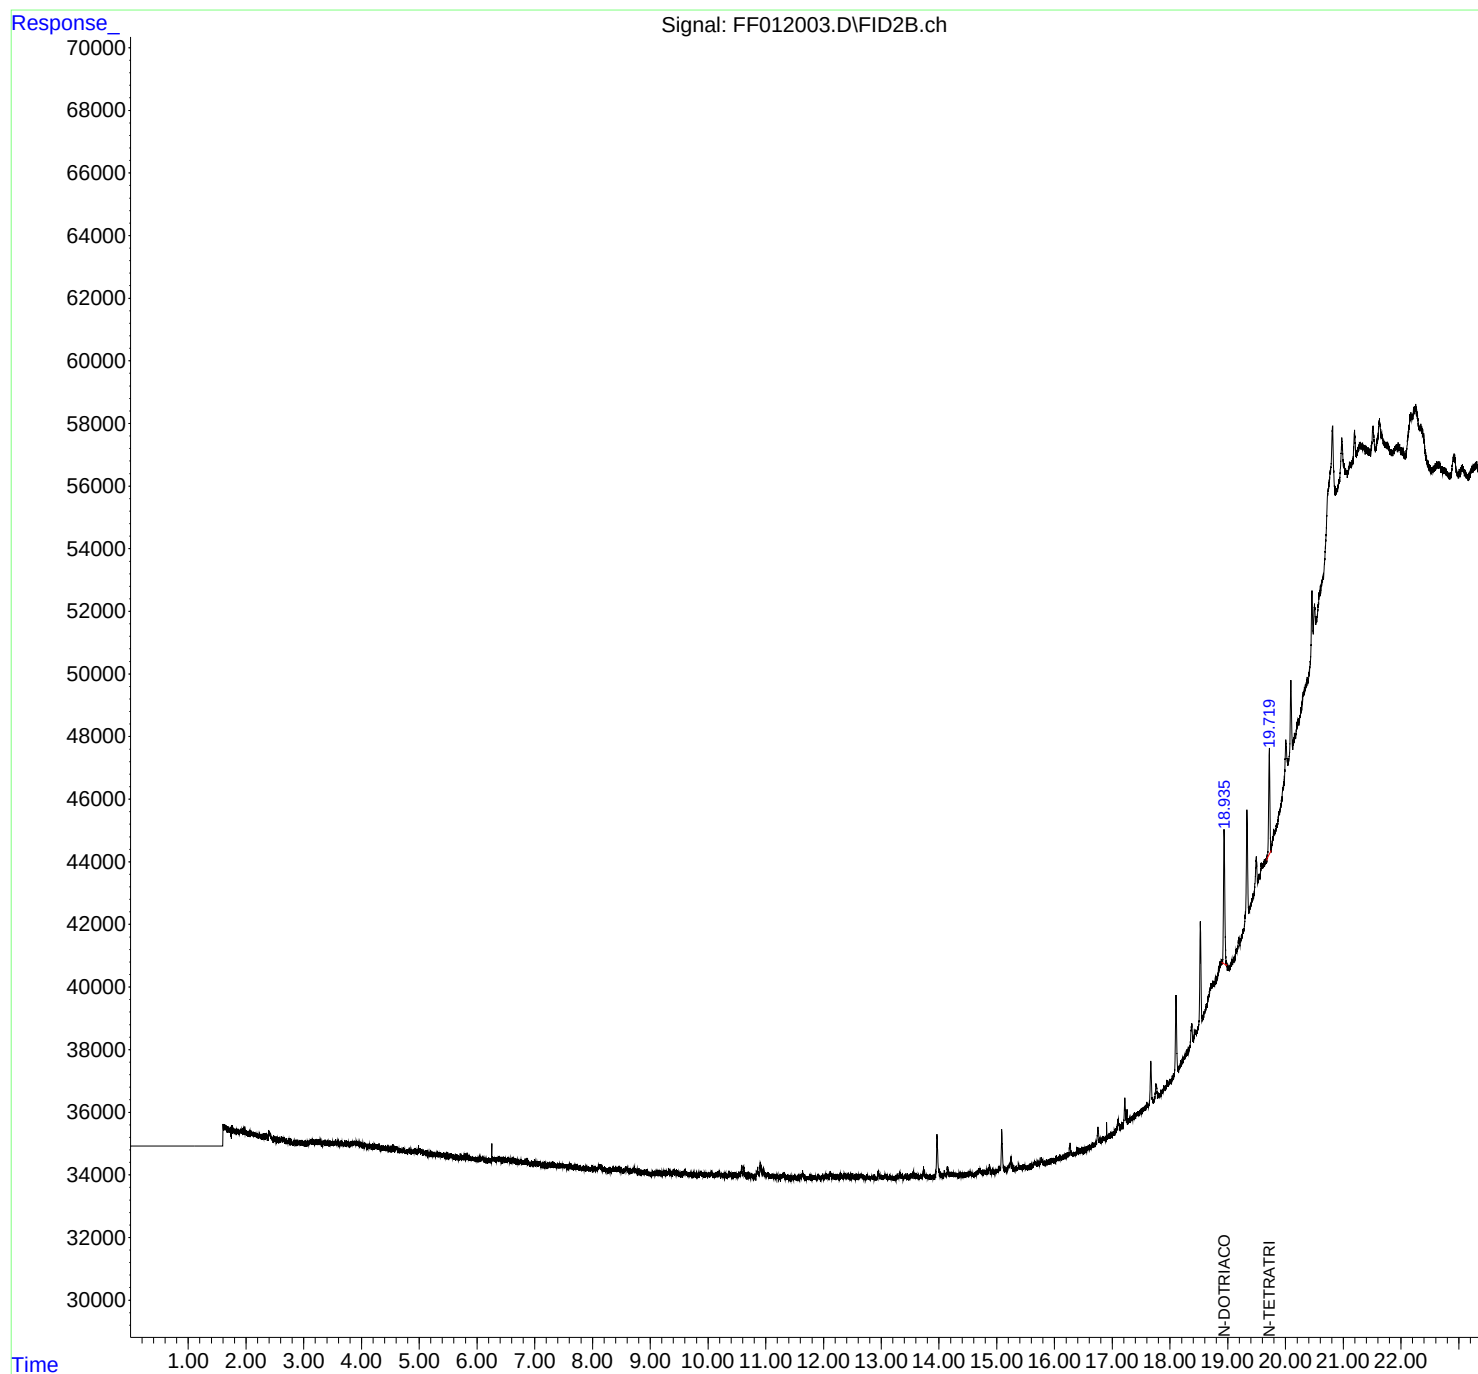


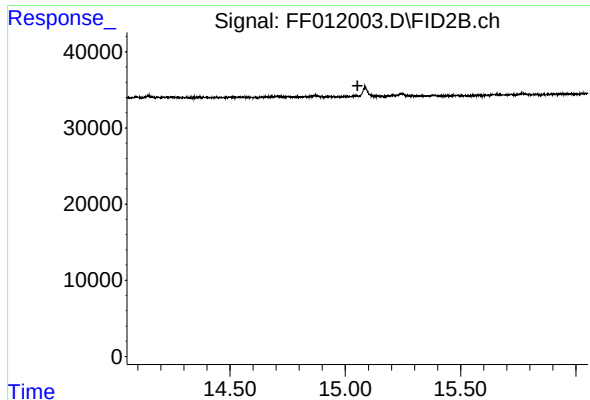

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

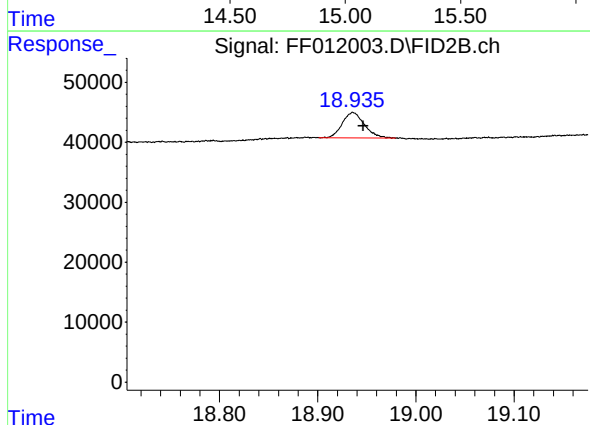

#14 N-DOTRIACONTANE

R.T.: 18.936 min
Delta R.T.: -0.011 min
Response: 66111
Conc: 0.51 ug/ml

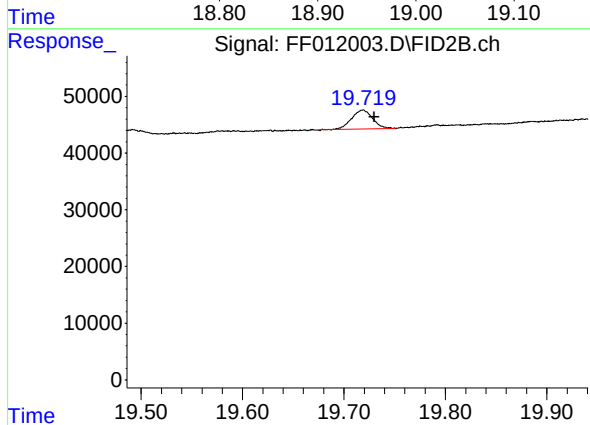

#15 N-TETRATRIACONTANE

R.T.: 19.719 min
Delta R.T.: -0.011 min
Response: 48899
Conc: 0.44 ug/ml