

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
 Data File : FF012007.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2023 13:27
 Operator : YP\AJ
 Sample : PB150734BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 09 02:43:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.041	1880108	16.316 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.102	47938	0.371 ug/ml
14) N-DOTRIACONTANE	18.936	73786	0.567 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012007.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 13:27
Operator : YP\AJ
Sample : PB150734BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 09 02:43:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

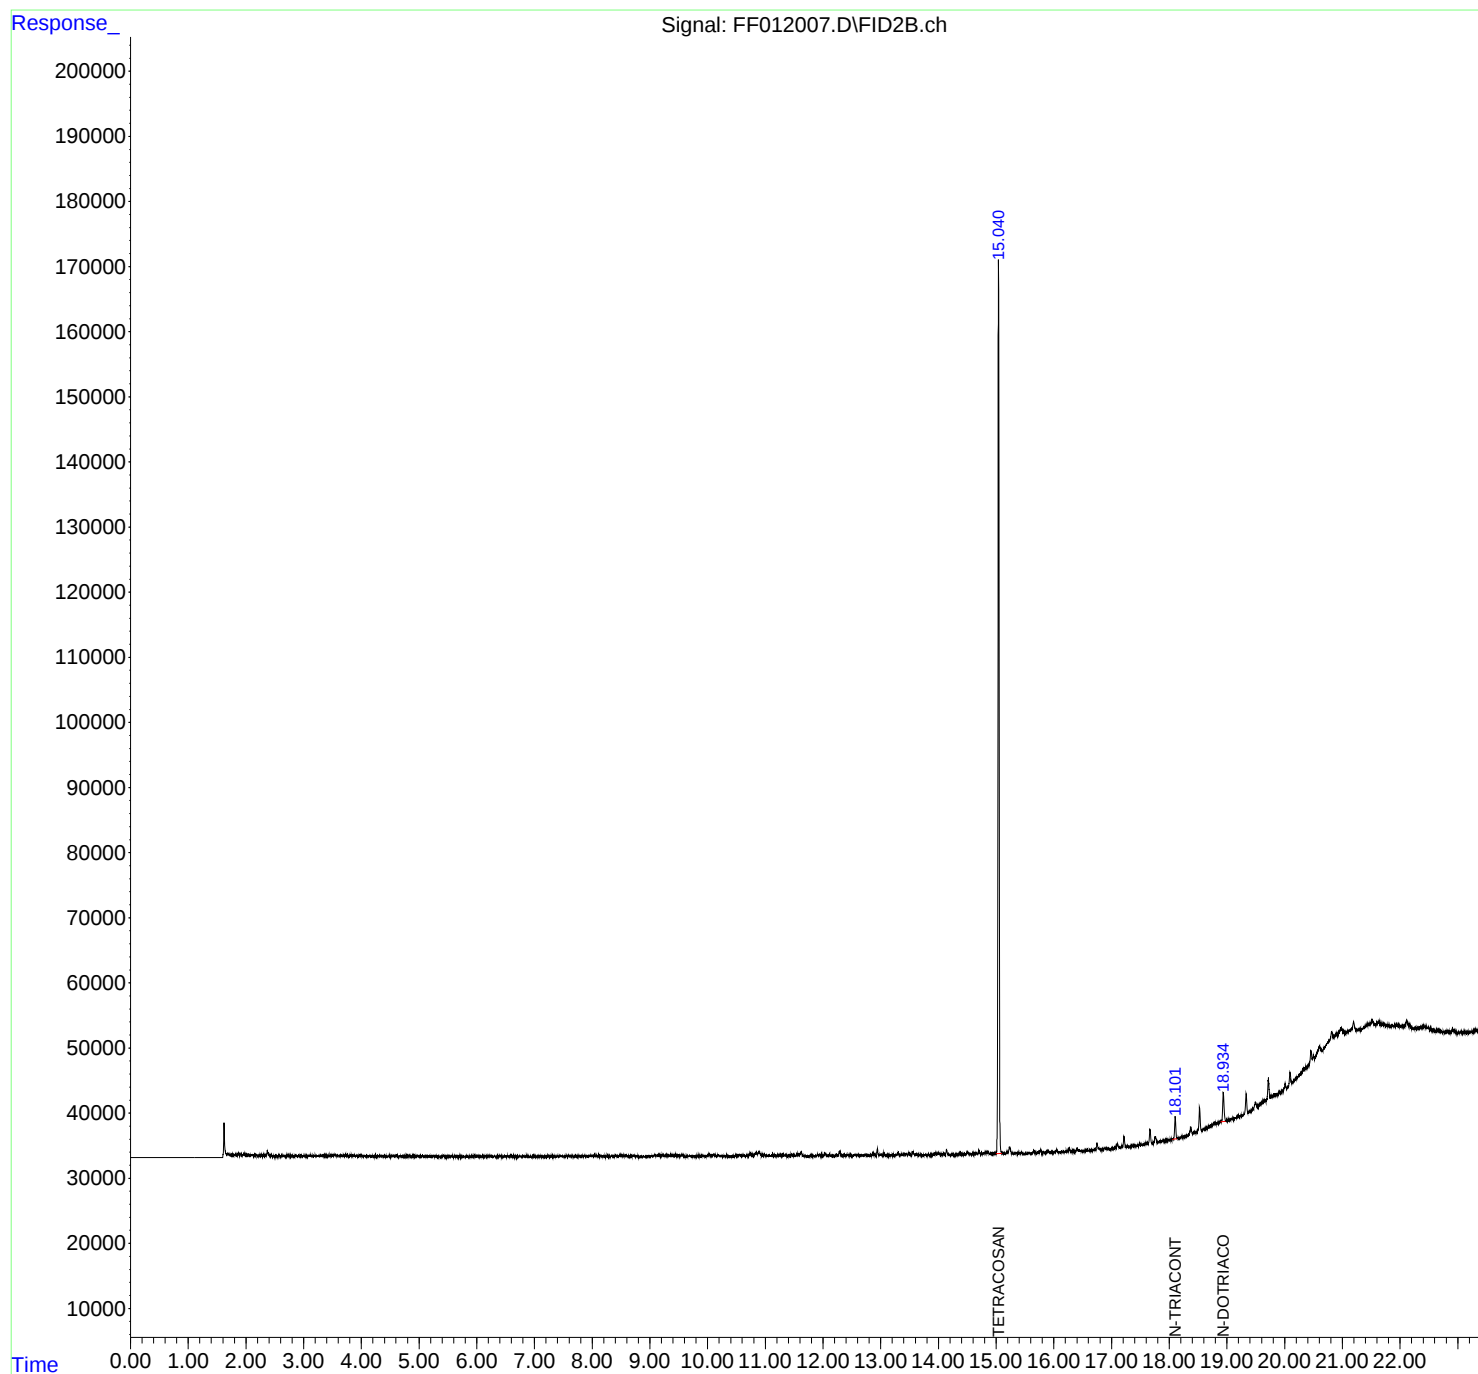

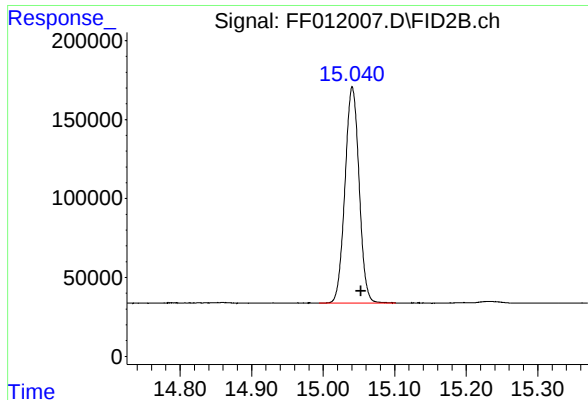


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.041 min
Delta R.T.: -0.012 min
Response: 1880108
Conc: 16.32 ug/ml

Instrument :


FID_F

ClientSampleId :

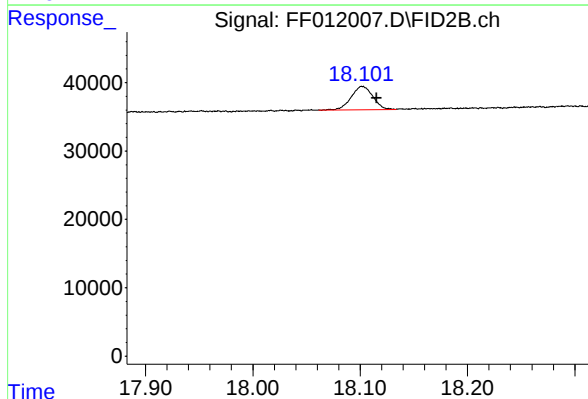

#13 N-TRIACONTANE

R.T.: 18.102 min
Delta R.T.: -0.013 min
Response: 47938
Conc: 0.37 ug/ml

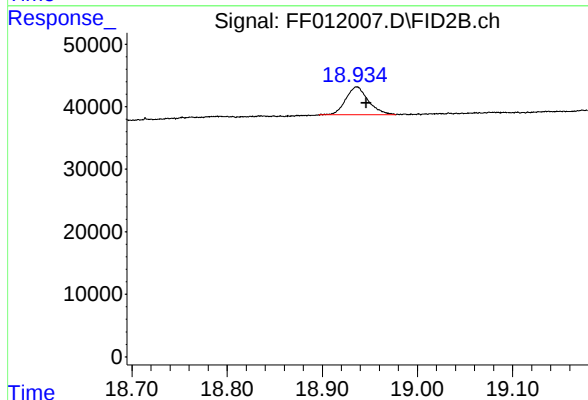

#14 N-DOTRIACONTANE

R.T.: 18.936 min
Delta R.T.: -0.010 min
Response: 73786
Conc: 0.57 ug/ml