

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
 Data File : FF012006.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2023 11:57
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Feb 09 02:43:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.764	2267776	18.931 ug/ml
12) N-OCTACOSANE	17.217	2216177	17.043 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012006.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 11:57
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Feb 09 02:43:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

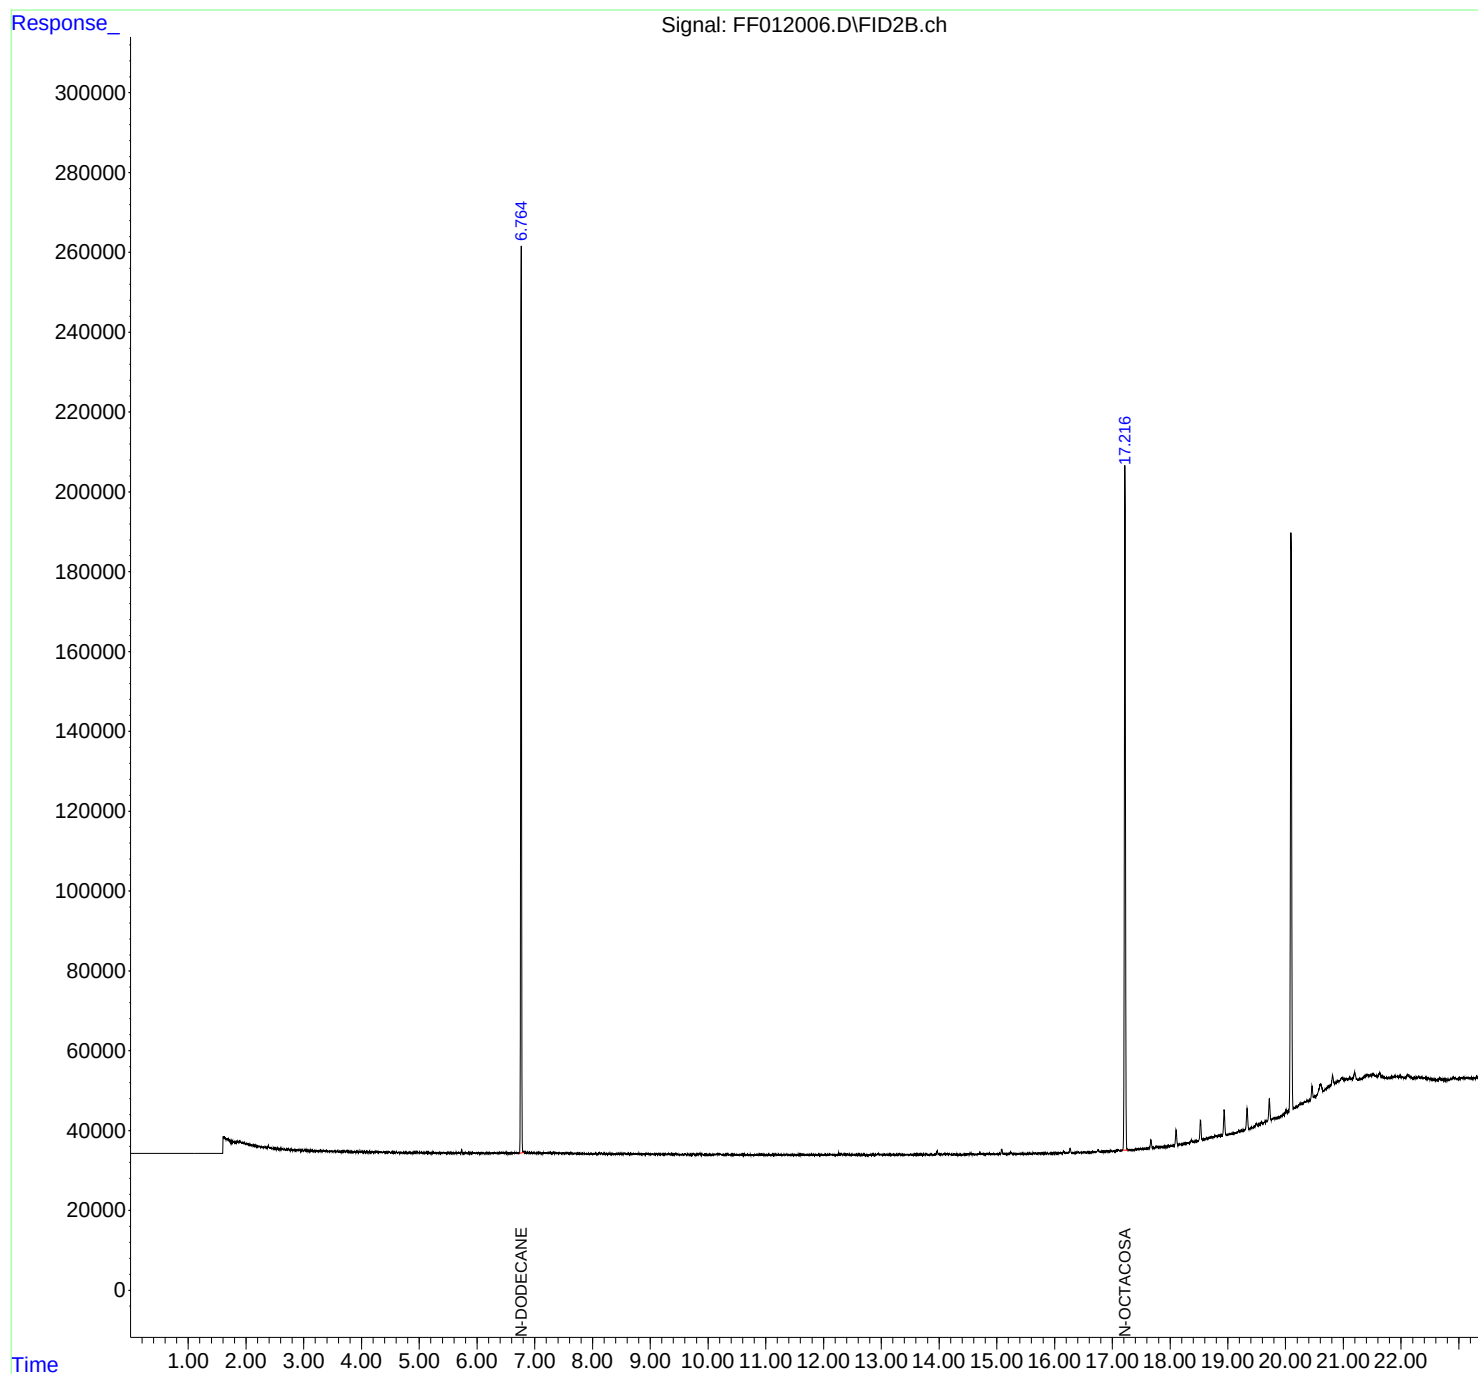


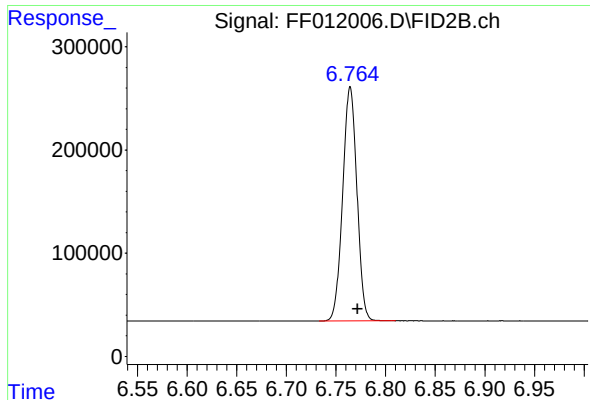

#3 N-DODECANE


R.T.: 6.764 min
Delta R.T.: -0.008 min
Response: 2267776
Conc: 18.93 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

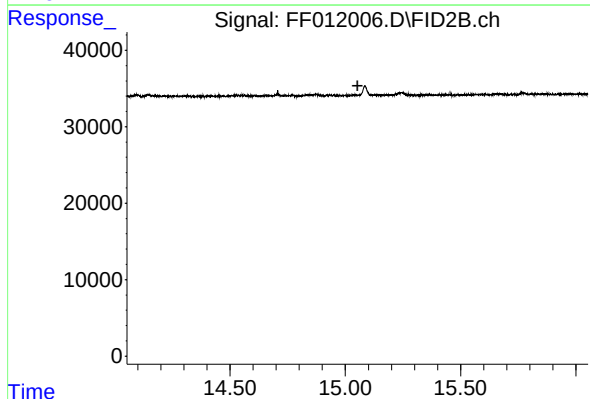

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

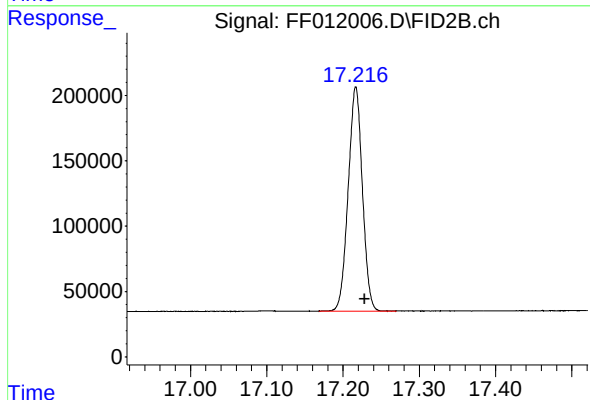

#12 N-OCTACOSANE

R.T.: 17.217 min
Delta R.T.: -0.012 min
Response: 2216177
Conc: 17.04 ug/ml