

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012014.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 17:24
Operator : YP\AJ
Sample : 01445-11 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JPP-34-020323

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Integration File: autoint1.e
Quant Time: Feb 09 02:44:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.051	98690	0.856 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020823\
Data File : FF012014.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2023 17:24
Operator : YP\AJ
Sample : 01445-11 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
JPP-34-020323


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Integration File: autoint1.e
Quant Time: Feb 09 02:44:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

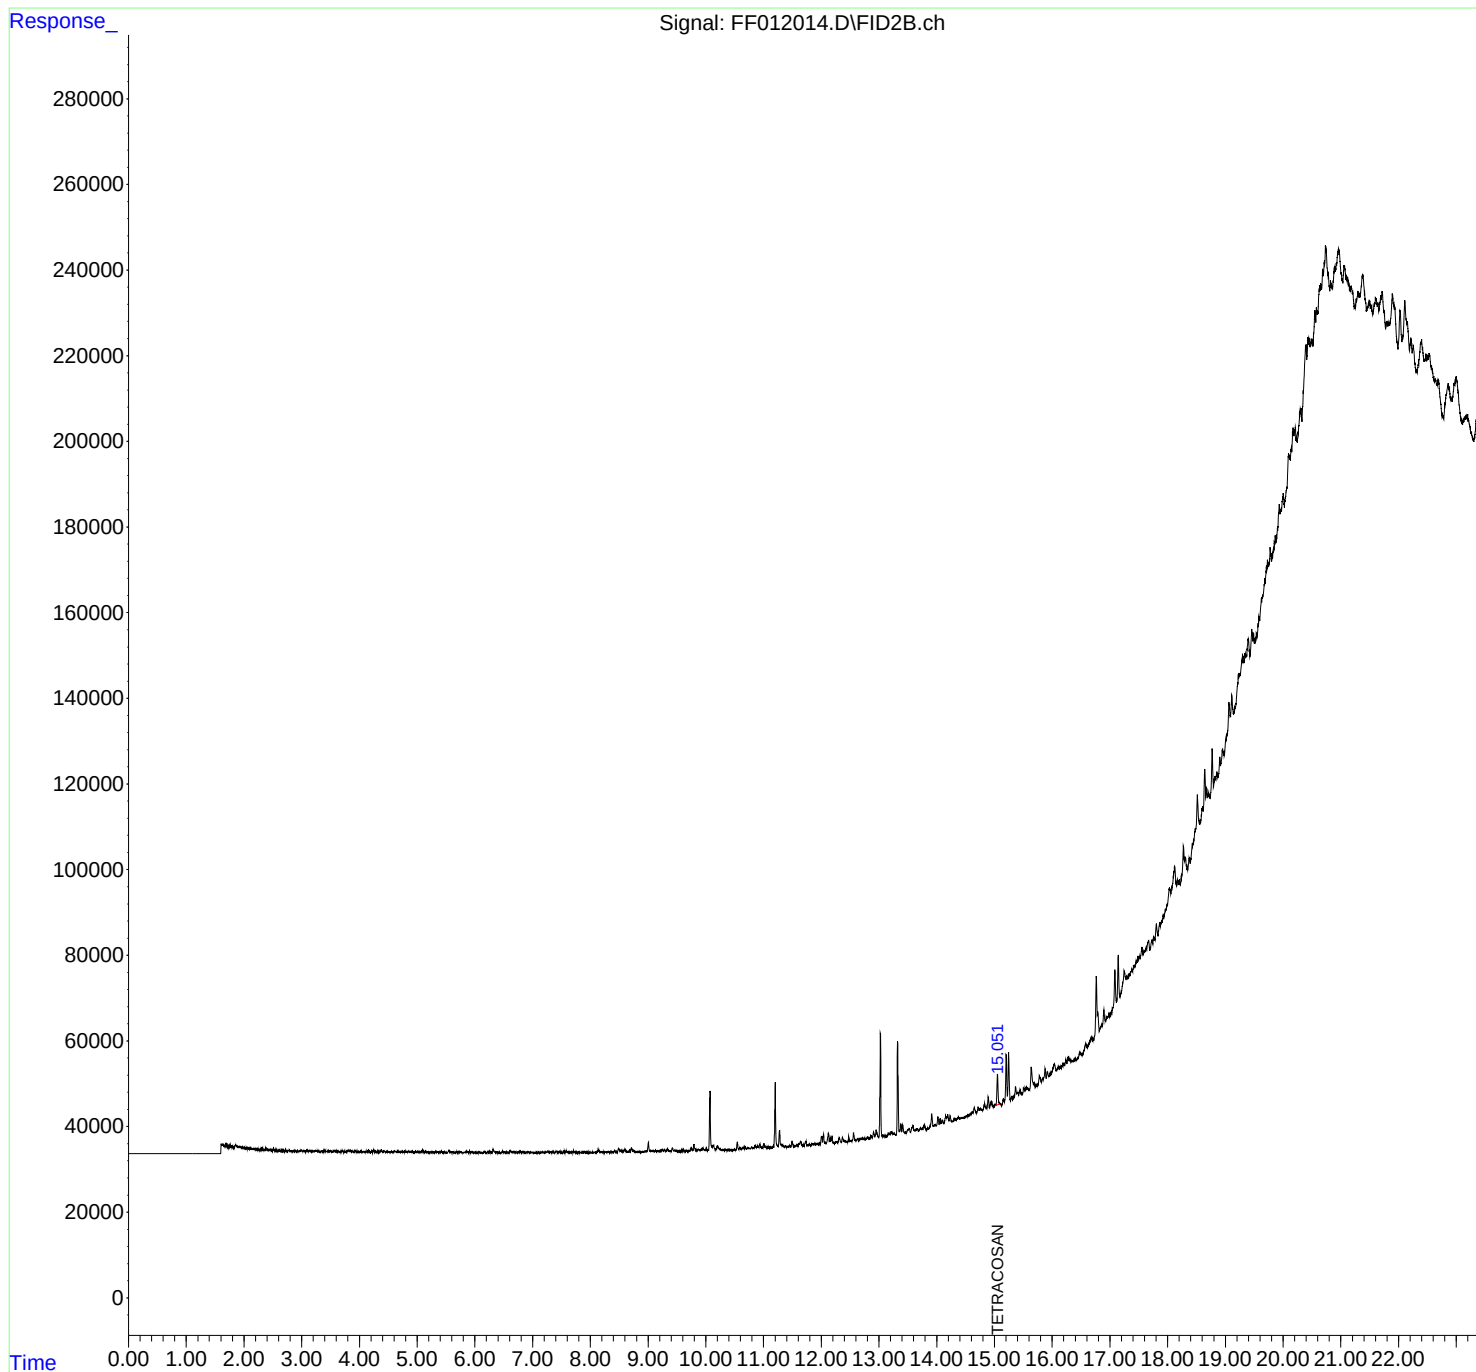

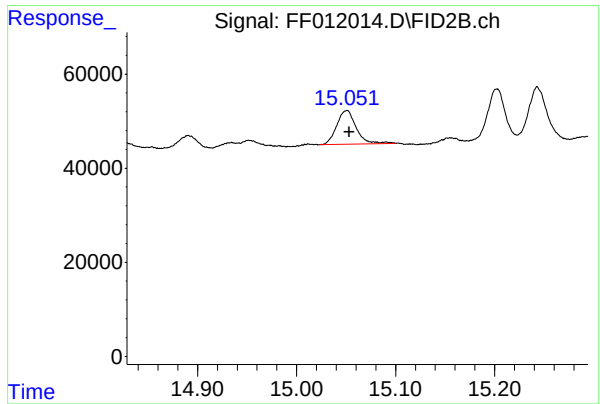

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.051 min
Delta R.T.: -0.002 min
Response: 98690
Conc: 0.86 ug/ml

Instrument :

FID_F

ClientSampleId :

JPP-34-020323

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 02/09/2023

Supervised By :Sohil Jodhani 02/09/2023