

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020824\
 Data File : FF013997.D
 Signal(s) : FID2B.ch
 Acq On : 08 Feb 2024 09:30
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 08 11:40:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020124.M
 Quant Title :
 QLast Update : Thu Feb 01 14:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.668	1809583	17.117 ug/ml
12)	N-OCTACOSANE	17.128	1899078	18.609 ug/ml
13)	N-TRIACONTANE	18.017	135571	1.353 ug/ml
14)	N-DOTRIACONTANE	18.851	199375	2.067 ug/ml
15)	N-TETRATRIACONTANE	19.634	159391	2.077 ug/ml
16)	N-HEXATRIACONTANE	20.377	111589	1.925 ug/ml
17)	N-OCTATRIACONTANE	21.108	136245	2.922 ug/ml
18)	N-TETRACONTANE	22.001	181069	4.261 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020824\
Data File : FF013997.D
Signal(s) : FID2B.ch
Acq On : 08 Feb 2024 09:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 08 11:40:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020124.M
Quant Title :
QLast Update : Thu Feb 01 14:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

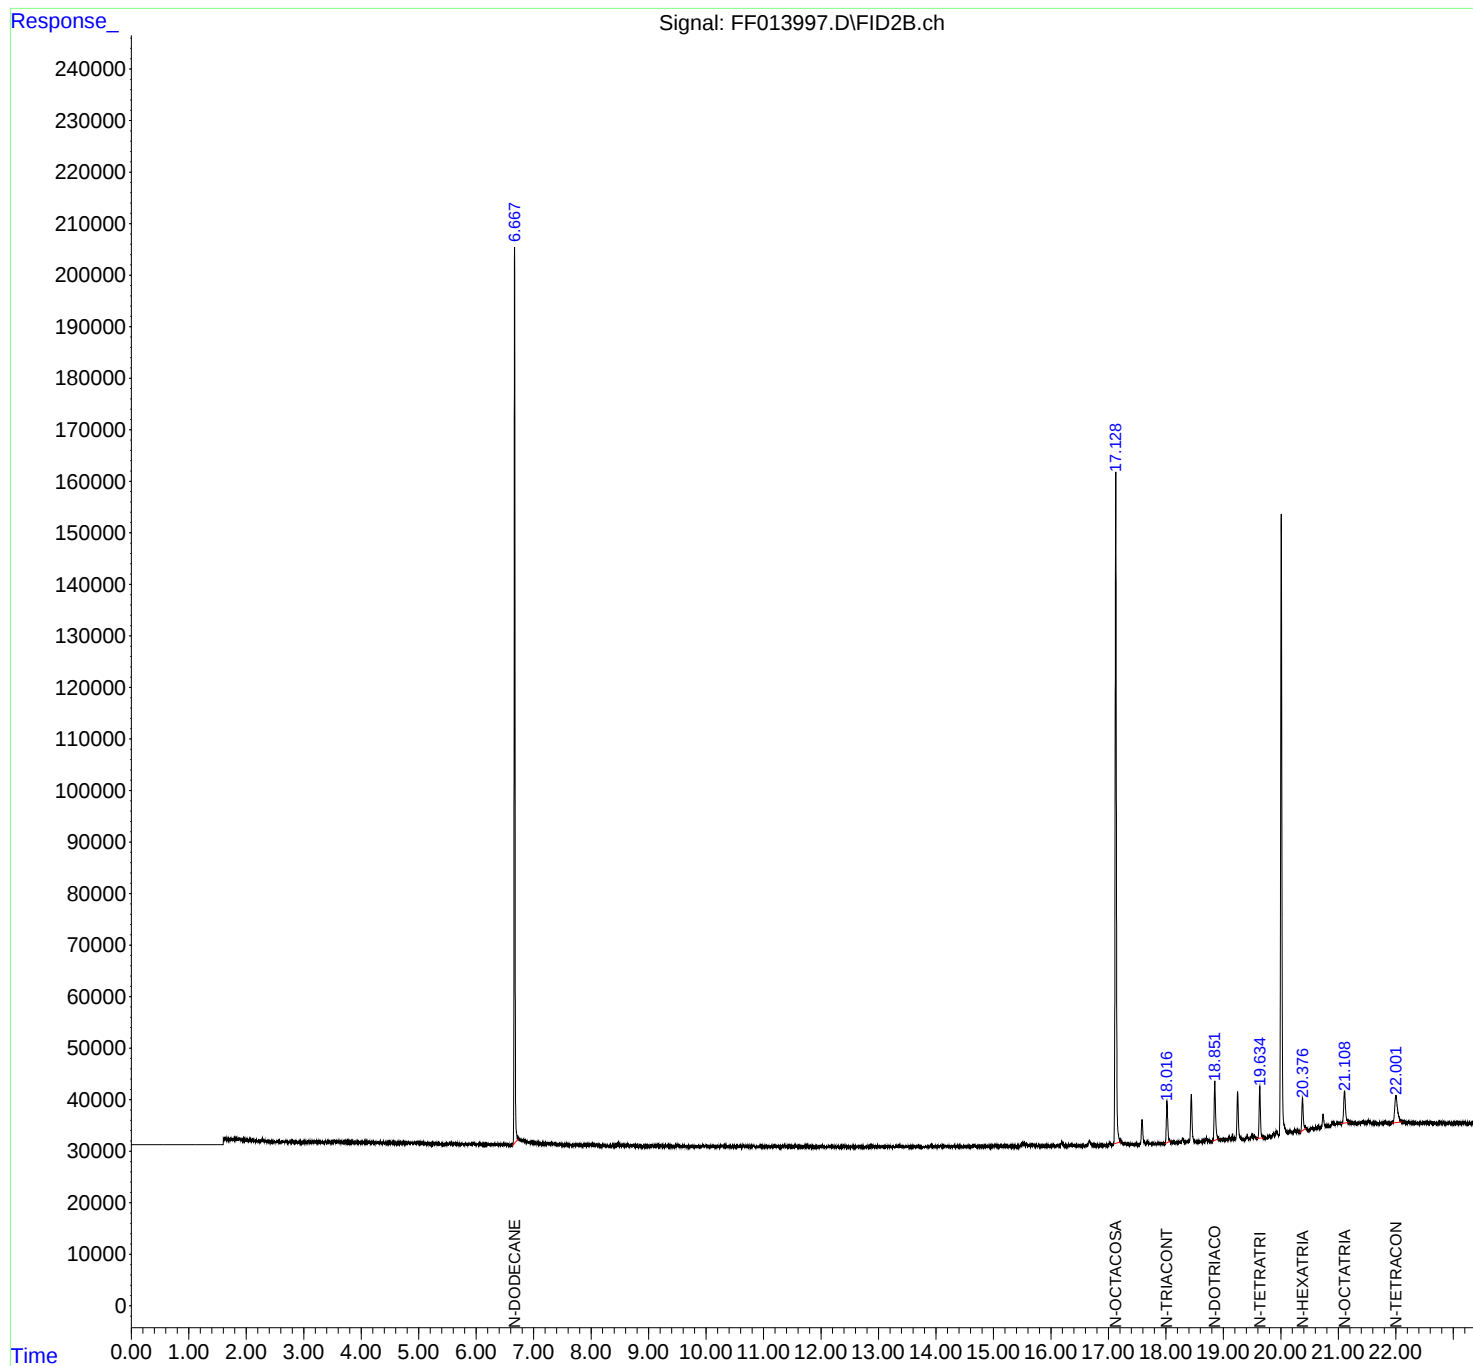


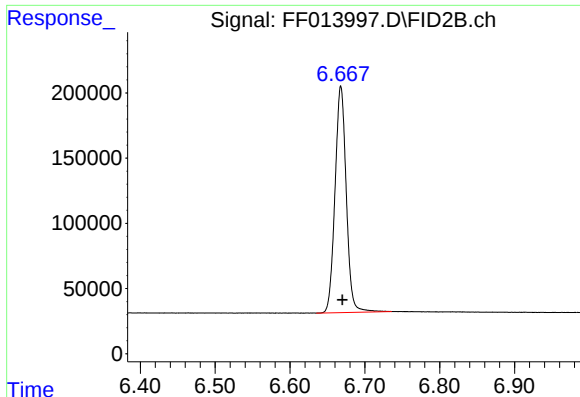

#3 N-DODECANE


R.T.: 6.668 min
Delta R.T.: -0.002 min
Response: 1809583
Conc: 17.12 ug/ml

Instrument :
FID_F
ClientSampleId :

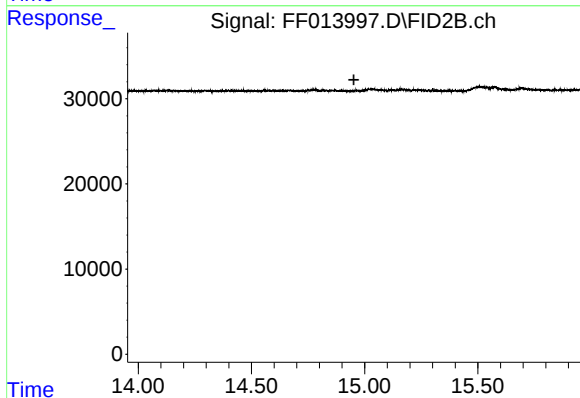


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.953 min
Response: 0
Conc: N.D.

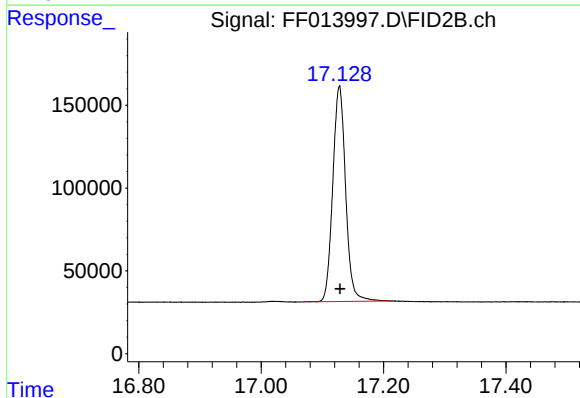


#12 N-OCTACOSANE

R.T.: 17.128 min
Delta R.T.: -0.001 min
Response: 1899078
Conc: 18.61 ug/ml

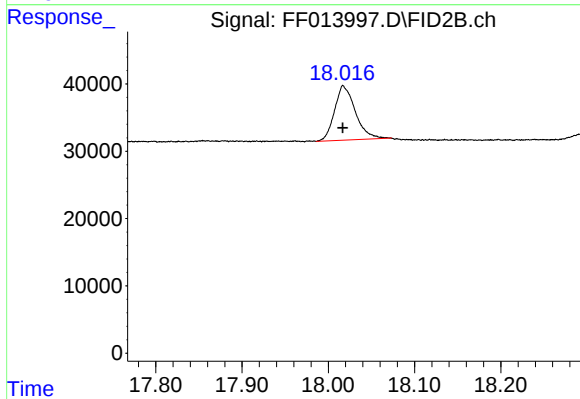

#13 N-TRIACONTANE


R.T.: 18.017 min
Delta R.T.: 0.000 min
Response: 135571
Conc: 1.35 ug/ml

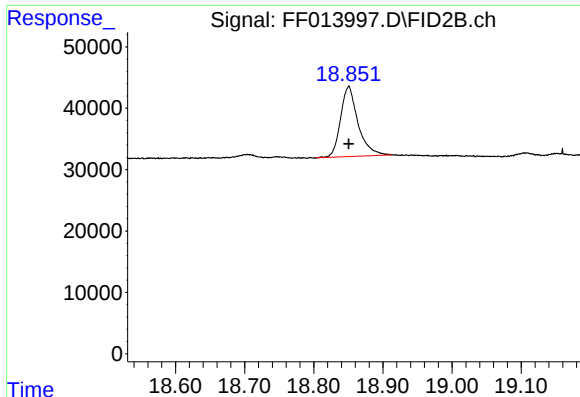

#14 N-DOTRIACONTANE


R.T.: 18.851 min
Delta R.T.: 0.000 min
Response: 199375
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :

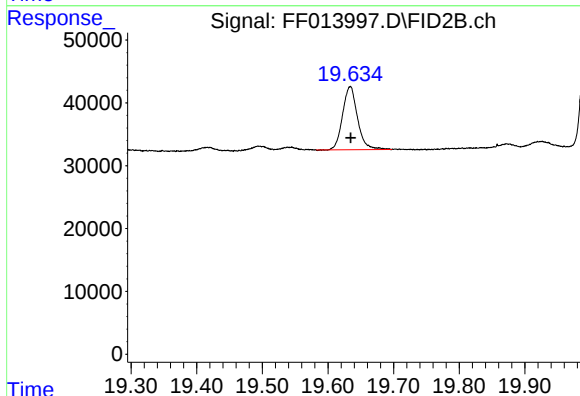


#15 N-TETRATRIACONTANE

R.T.: 19.634 min
Delta R.T.: 0.000 min
Response: 159391
Conc: 2.08 ug/ml

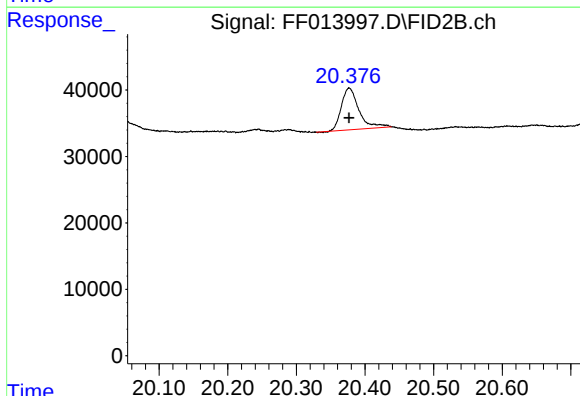


#16 N-HEXATRIACONTANE

R.T.: 20.377 min
Delta R.T.: 0.000 min
Response: 111589
Conc: 1.93 ug/ml

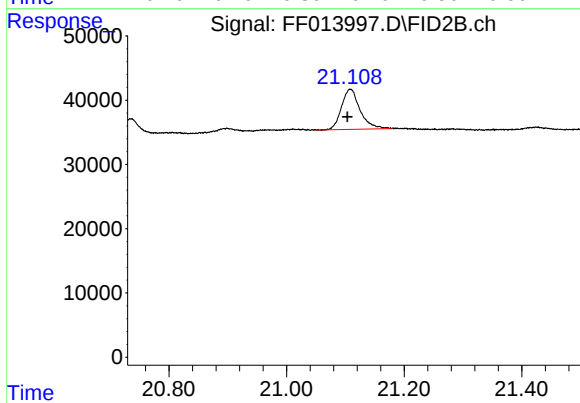

#17 N-OCTATRIACONTANE

R.T.: 21.108 min
Delta R.T.: 0.005 min
Response: 136245
Conc: 2.92 ug/ml

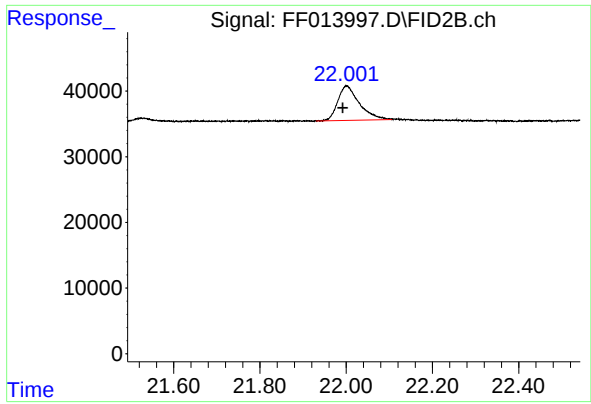

#18 N-TETRACONTANE

R.T.: 22.001 min
Delta R.T.: 0.009 min
Response: 181069
Conc: 4.26 ug/ml

Instrument :
FID_F
ClientSampleId :