

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020923\  
 Data File : FF012023.D  
 Signal(s) : FID2B.ch  
 Acq On : 09 Feb 2023 10:40  
 Operator : YP\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Feb 09 22:43:20 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
 Quant Title :  
 QLast Update : Fri Jan 27 14:21:25 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.769	1985488	16.575 ug/ml
12) N-OCTACOSANE	17.229	1901013	14.619 ug/ml
13) N-TRIACONTANE	18.115	53799	0.417 ug/ml
14) N-DOTRIACONTANE	18.948	100381	0.771 ug/ml
15) N-TETRATRIACONTANE	19.731	114093	1.025 ug/ml
16) N-HEXATRIACONTANE	20.471	207525	2.020 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020923\  
 Data File : FF012023.D  
 Signal(s) : FID2B.ch  
 Acq On : 09 Feb 2023 10:40  
 Operator : YP\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Feb 09 22:43:20 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
 Quant Title :  
 QLast Update : Fri Jan 27 14:21:25 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

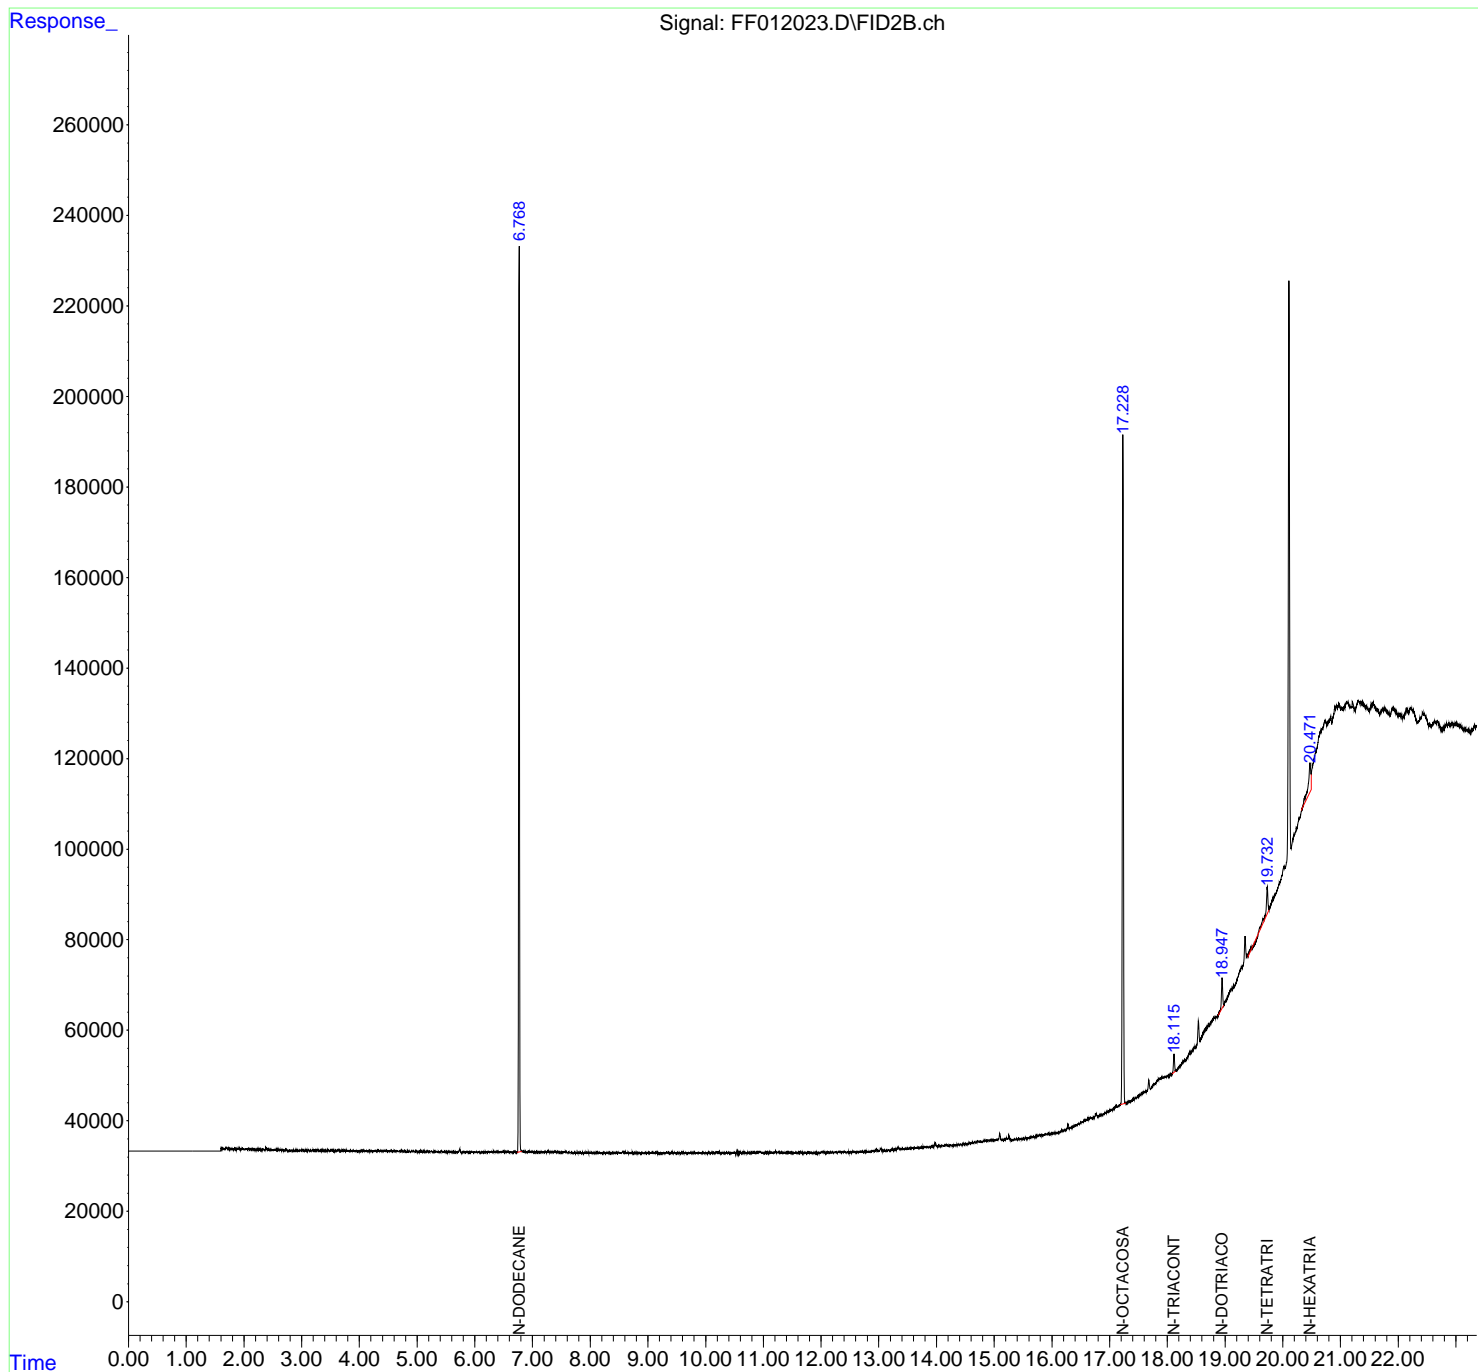


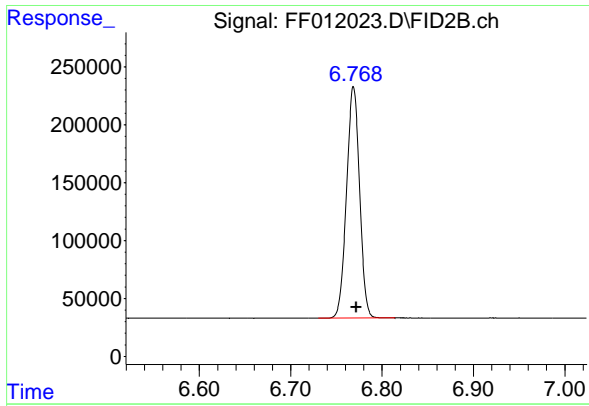

#3 N-DODECANE


R.T.: 6.769 min  
 Delta R.T.: -0.003 min  
 Response: 1985488  
 Conc: 16.57 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :

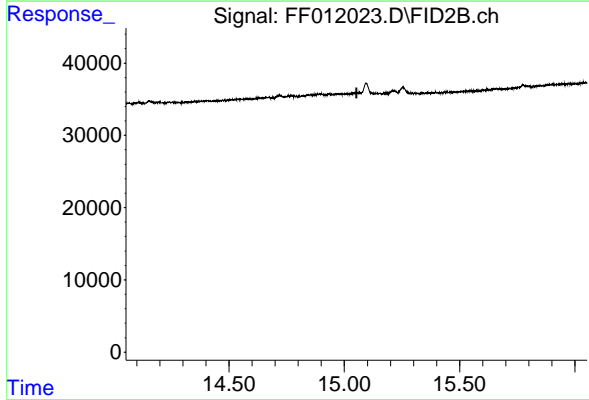


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
 Exp R.T. : 15.053 min  
 Response: 0  
 Conc: N.D.

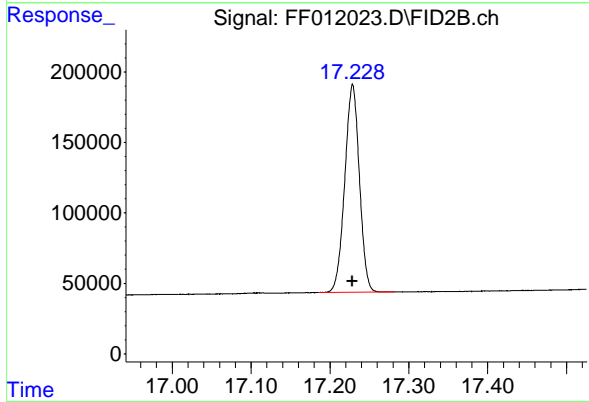


#12 N-OCTACOSANE

R.T.: 17.229 min  
 Delta R.T.: 0.000 min  
 Response: 1901013  
 Conc: 14.62 ug/ml

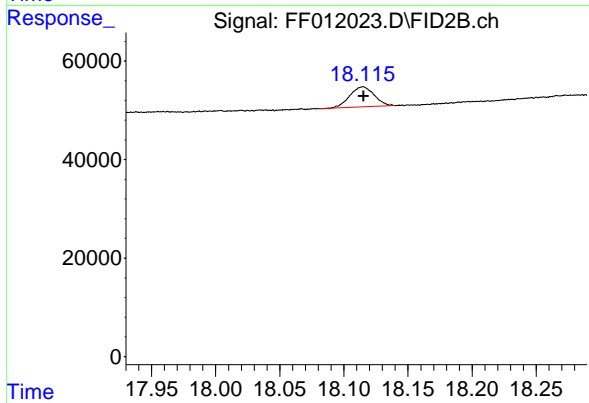

#13 N-TRIACONTANE


R.T.: 18.115 min  
 Delta R.T.: 0.000 min  
 Response: 53799  
 Conc: 0.42 ug/ml

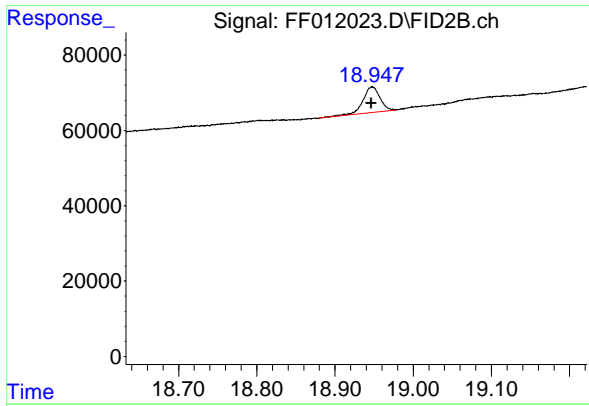

#14 N-DOTRIACONTANE


R.T.: 18.948 min  
 Delta R.T.: 0.002 min  
 Response: 100381  
 Conc: 0.77 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :

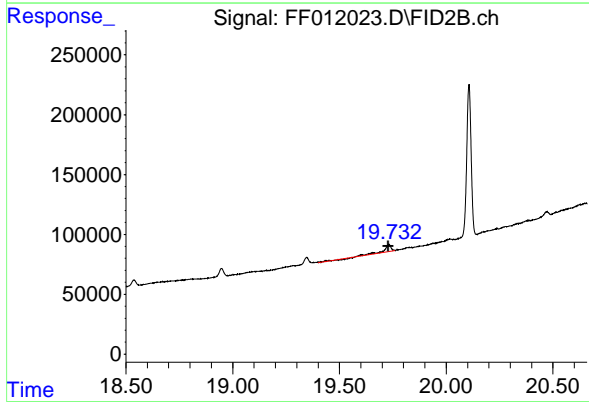

#15 N-TETRATRIACONTANE

R.T.: 19.731 min  
 Delta R.T.: 0.001 min  
 Response: 114093  
 Conc: 1.02 ug/ml

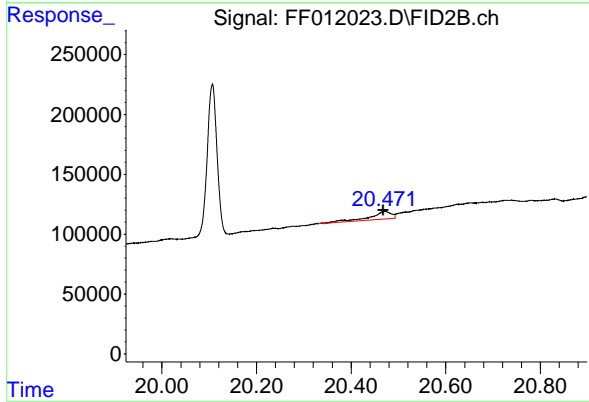

#16 N-HEXATRIACONTANE

R.T.: 20.471 min  
 Delta R.T.: 0.003 min  
 Response: 207525  
 Conc: 2.02 ug/ml