

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020923\  
Data File : FF012027.D  
Signal(s) : FID2B.ch  
Acq On : 09 Feb 2023 12:38  
Operator : YP\AJ  
Sample : 01445-03 20X  
Misc :  
ALS Vial : 58 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
JPP-26-020323

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023  
Supervised By :Sohil Jodhani 02/10/2023

Integration File: autoint1.e  
Quant Time: Feb 09 22:43:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
Quant Title :  
QLast Update : Fri Jan 27 14:21:25 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.053 | 67008    | 0.582 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020923\  
Data File : FF012027.D  
Signal(s) : FID2B.ch  
Acq On : 09 Feb 2023 12:38  
Operator : YP\AJ  
Sample : 01445-03 20X  
Misc :  
ALS Vial : 58 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
JPP-26-020323


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023  
Supervised By :Sohil Jodhani 02/10/2023

Integration File: autoint1.e  
Quant Time: Feb 09 22:43:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
Quant Title :  
QLast Update : Fri Jan 27 14:21:25 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

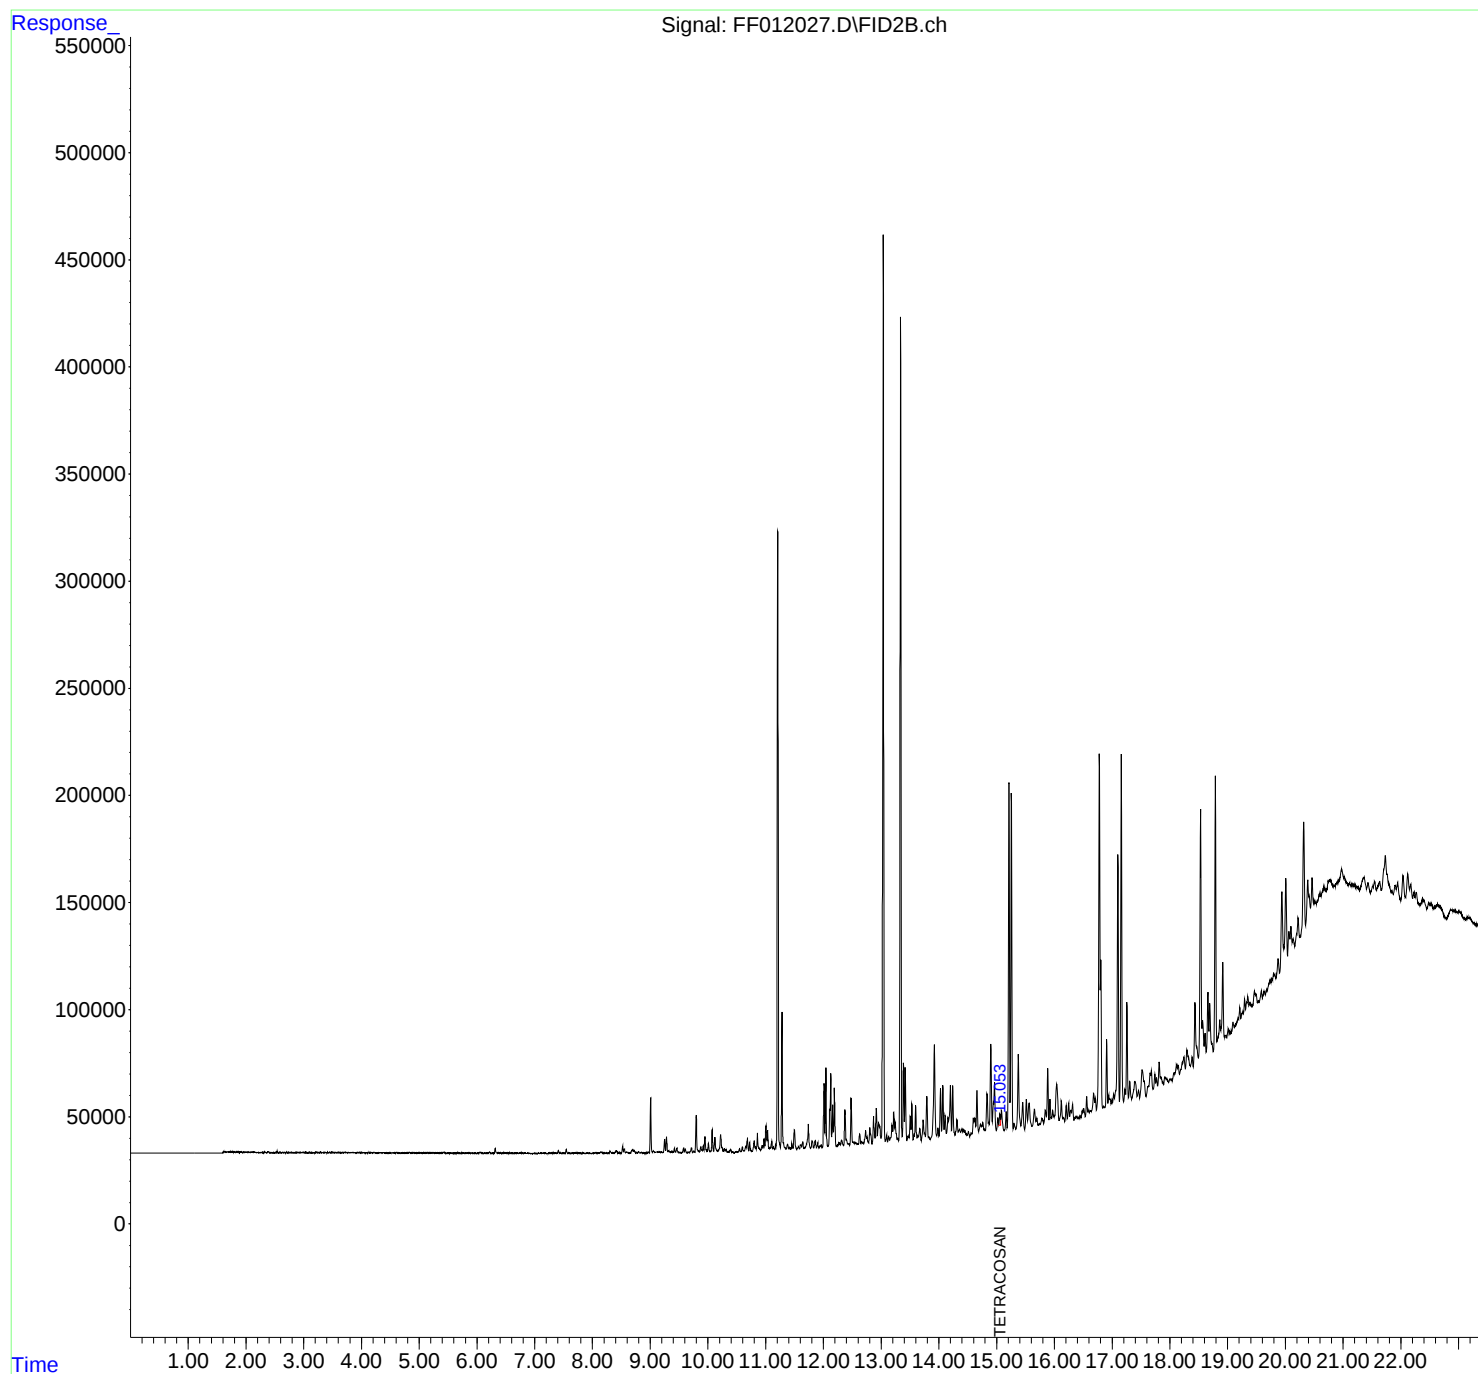

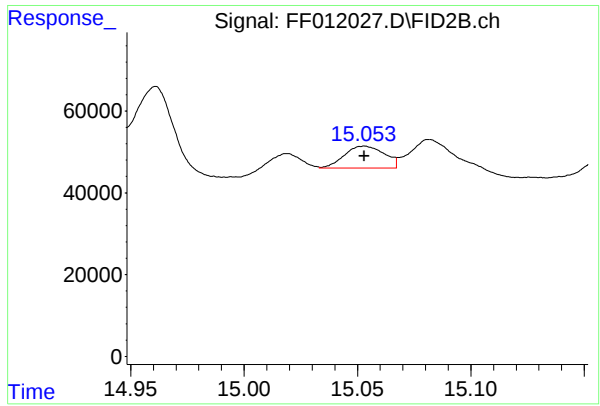

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min  
Delta R.T.: 0.000 min  
Response: 67008  
Conc: 0.58 ug/ml

Instrument :

FID\_F

ClientSampleId :

JPP-26-020323

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 02/10/2023

Supervised By :Sohil Jodhani 02/10/2023