

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021020\
Data File : FF006372.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2020 20:25
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 11 04:48:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 04:47:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) N-HEXATRIACONTANE	20.038	154724	1.557 ug/ml
18) N-TETRACONTANE	21.617	215015	3.046 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021020\
Data File : FF006372.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2020 20:25
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 11 04:48:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 04:47:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

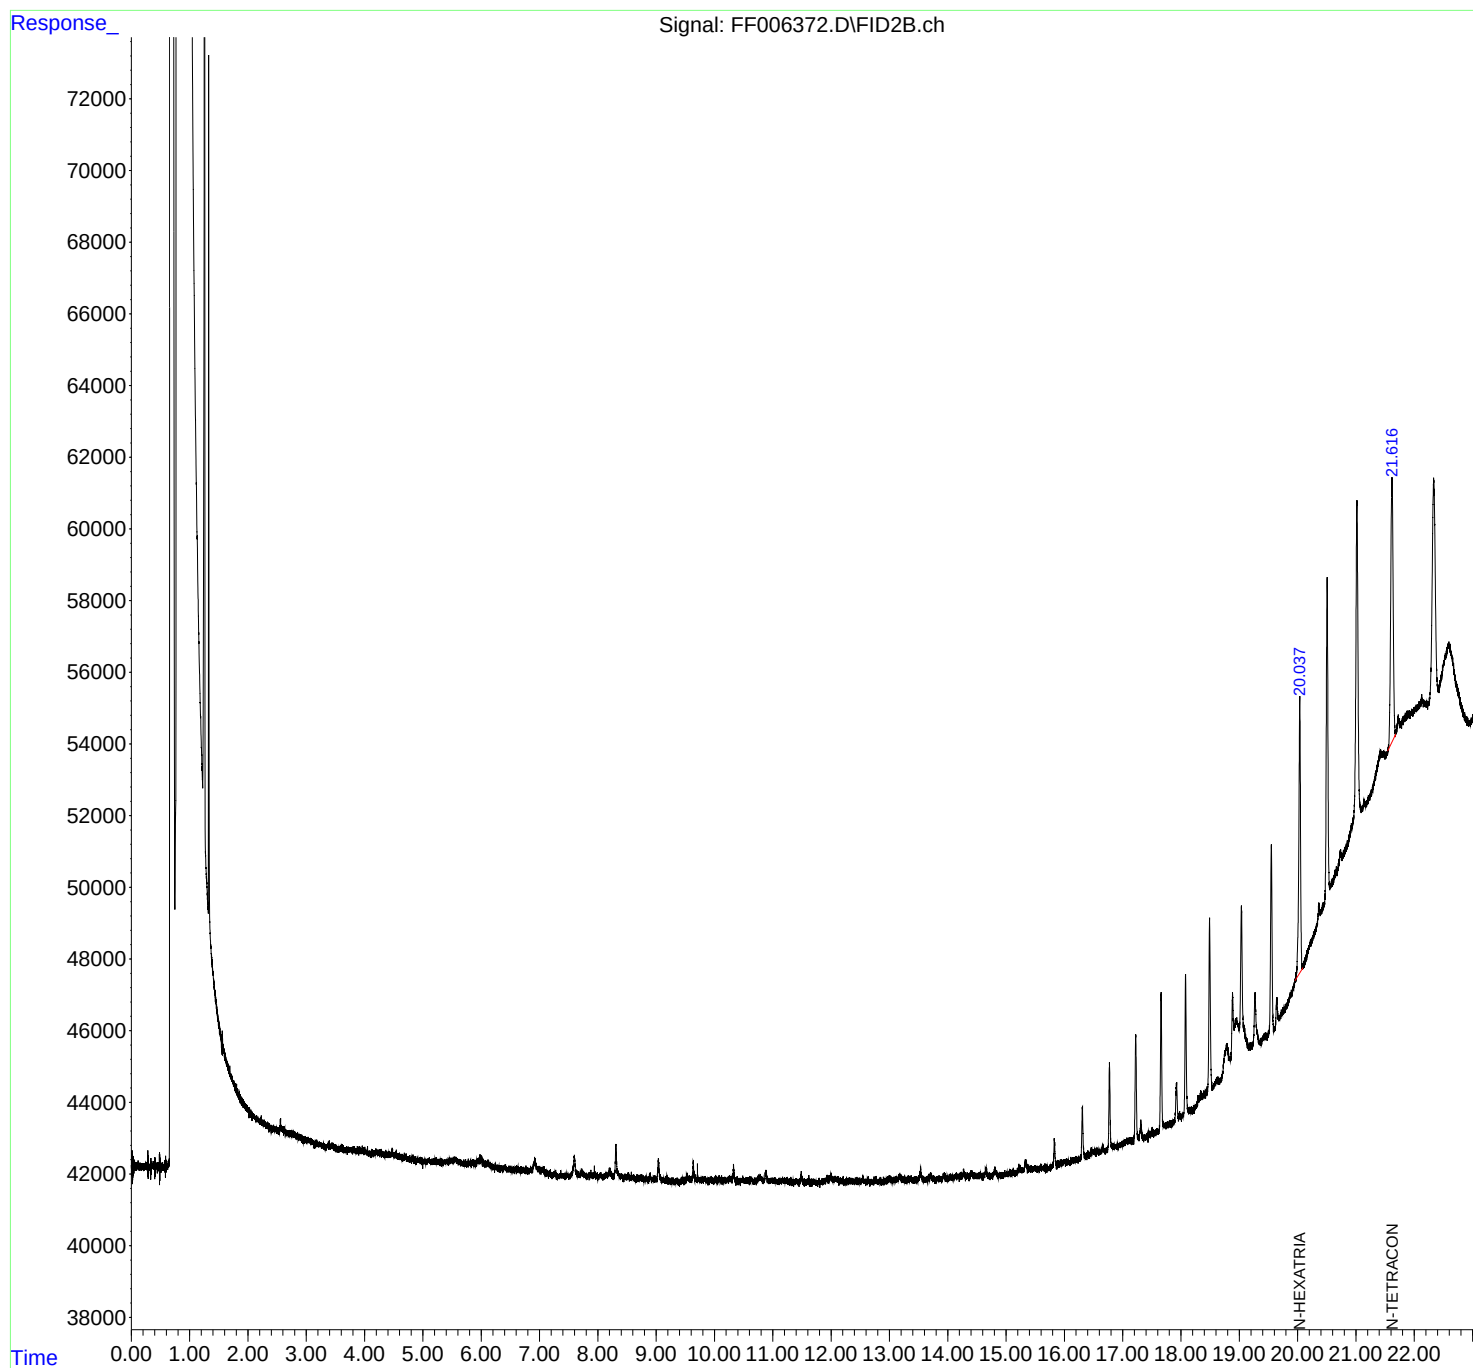


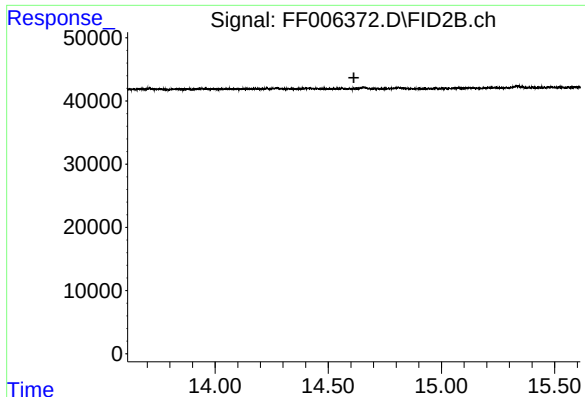

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.613 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

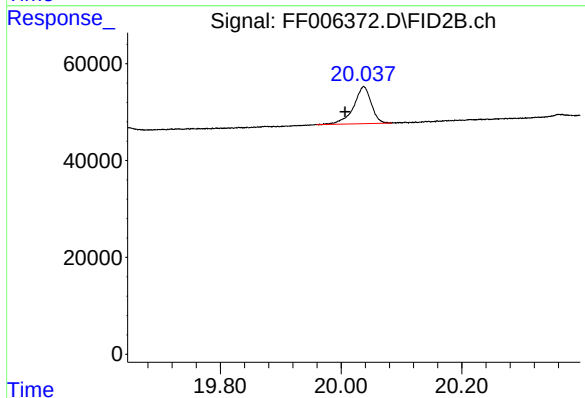

#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: 0.031 min
Response: 154724
Conc: 1.56 ug/ml

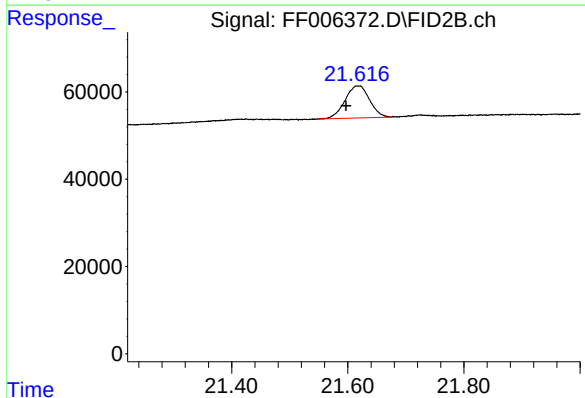

#18 N-TETRACONTANE

R.T.: 21.617 min
Delta R.T.: 0.020 min
Response: 215015
Conc: 3.05 ug/ml