

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
 Data File : FF012034.D
 Signal(s) : FID2B.ch
 Acq On : 10 Feb 2023 12:49
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 13 06:24:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.771	2149112	17.941 ug/ml
12) N-OCTACOSANE	17.234	2113399	16.252 ug/ml
13) N-TRIACONTANE	18.121	108902	0.844 ug/ml
14) N-DOTRIACONTANE	18.953	139974	1.076 ug/ml
15) N-TETRATRIACONTANE	19.737	179871	1.616 ug/ml
16) N-HEXATRIACONTANE	20.479	204178	1.988 ug/ml
17) N-OCTATRIACONTANE	21.224	307507	3.122 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
Data File : FF012034.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2023 12:49
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 06:24:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

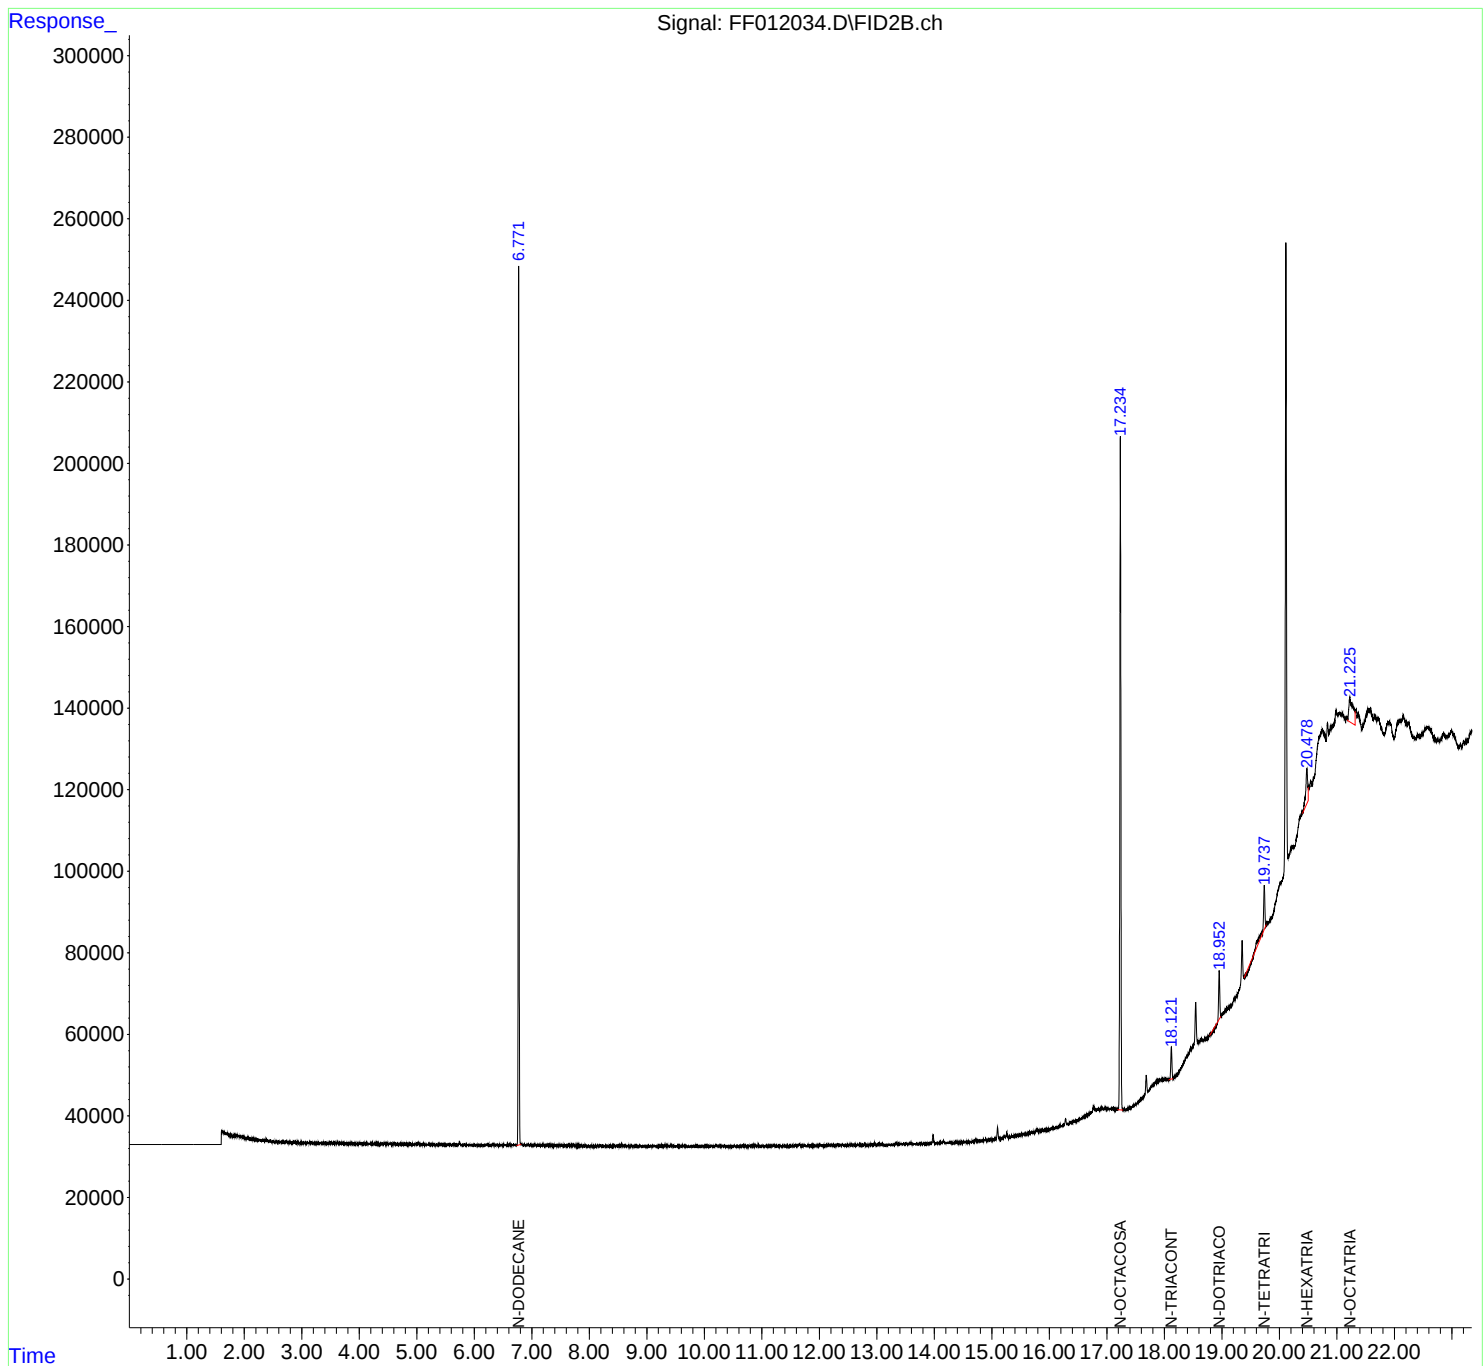


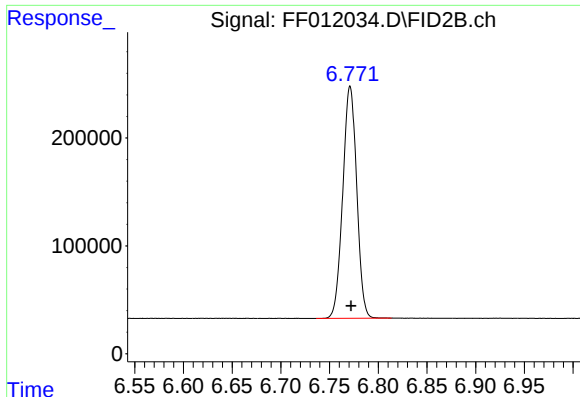

#3 N-DODECANE


R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 2149112
Conc: 17.94 ug/ml

Instrument :
FID_F
ClientSampleId :

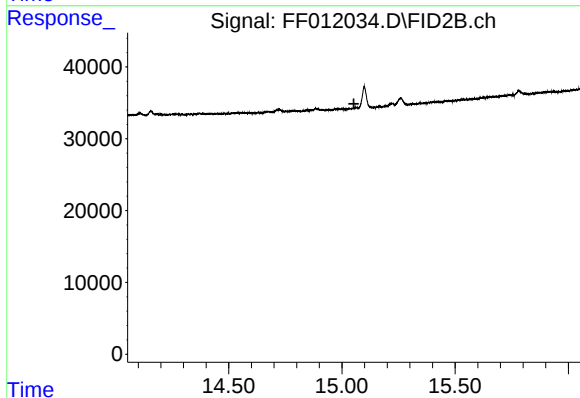


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

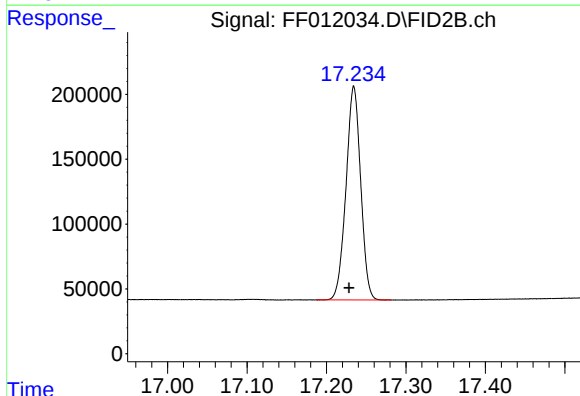


#12 N-OCTACOSANE

R.T.: 17.234 min
Delta R.T.: 0.006 min
Response: 2113399
Conc: 16.25 ug/ml

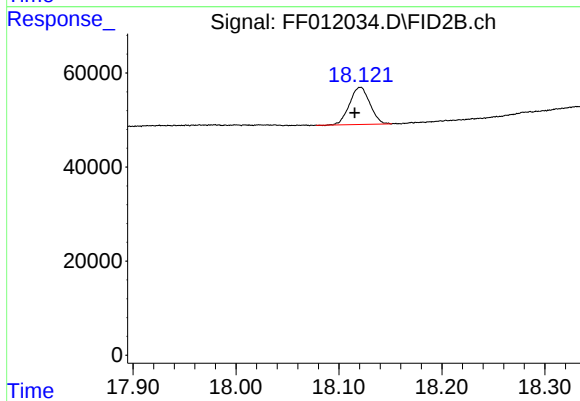

#13 N-TRIACONTANE


R.T.: 18.121 min
Delta R.T.: 0.006 min
Response: 108902
Conc: 0.84 ug/ml

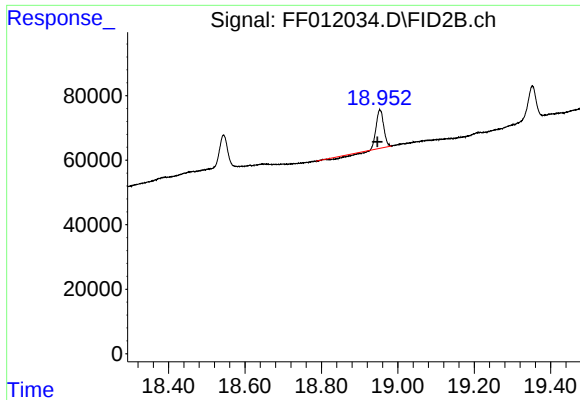

#14 N-DOTRIACONTANE


R.T.: 18.953 min
Delta R.T.: 0.007 min
Response: 139974
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

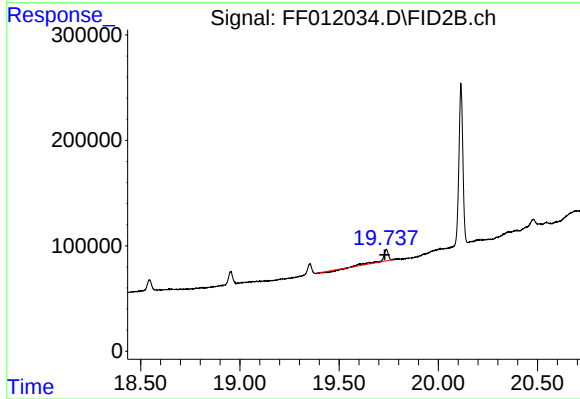


#15 N-TETRATRIACONTANE

R.T.: 19.737 min
Delta R.T.: 0.007 min
Response: 179871
Conc: 1.62 ug/ml

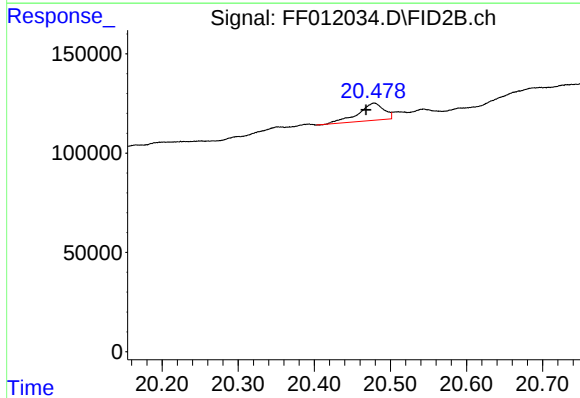

#16 N-HEXATRIACONTANE

R.T.: 20.479 min
Delta R.T.: 0.011 min
Response: 204178
Conc: 1.99 ug/ml

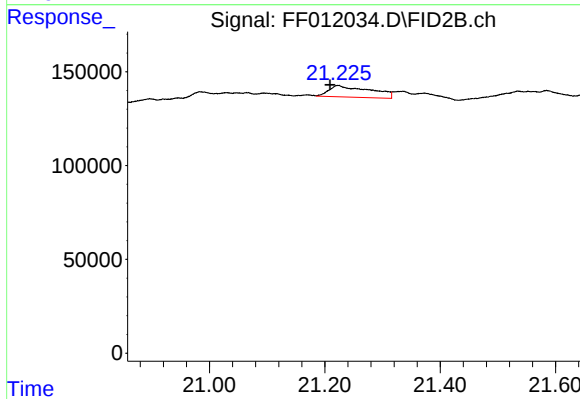

#17 N-OCTATRIACONTANE

R.T.: 21.224 min
Delta R.T.: 0.014 min
Response: 307507
Conc: 3.12 ug/ml