

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
Data File : FF012038.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2023 15:22
Operator : YP\AJ
Sample : 01510-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TWM-TP14-020823

Integration File: autoint1.e
Quant Time: Feb 13 06:25:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	1455967	12.635 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
Data File : FF012038.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2023 15:22
Operator : YP\AJ
Sample : 01510-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TWM-TP14-020823

Integration File: autoint1.e
Quant Time: Feb 13 06:25:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

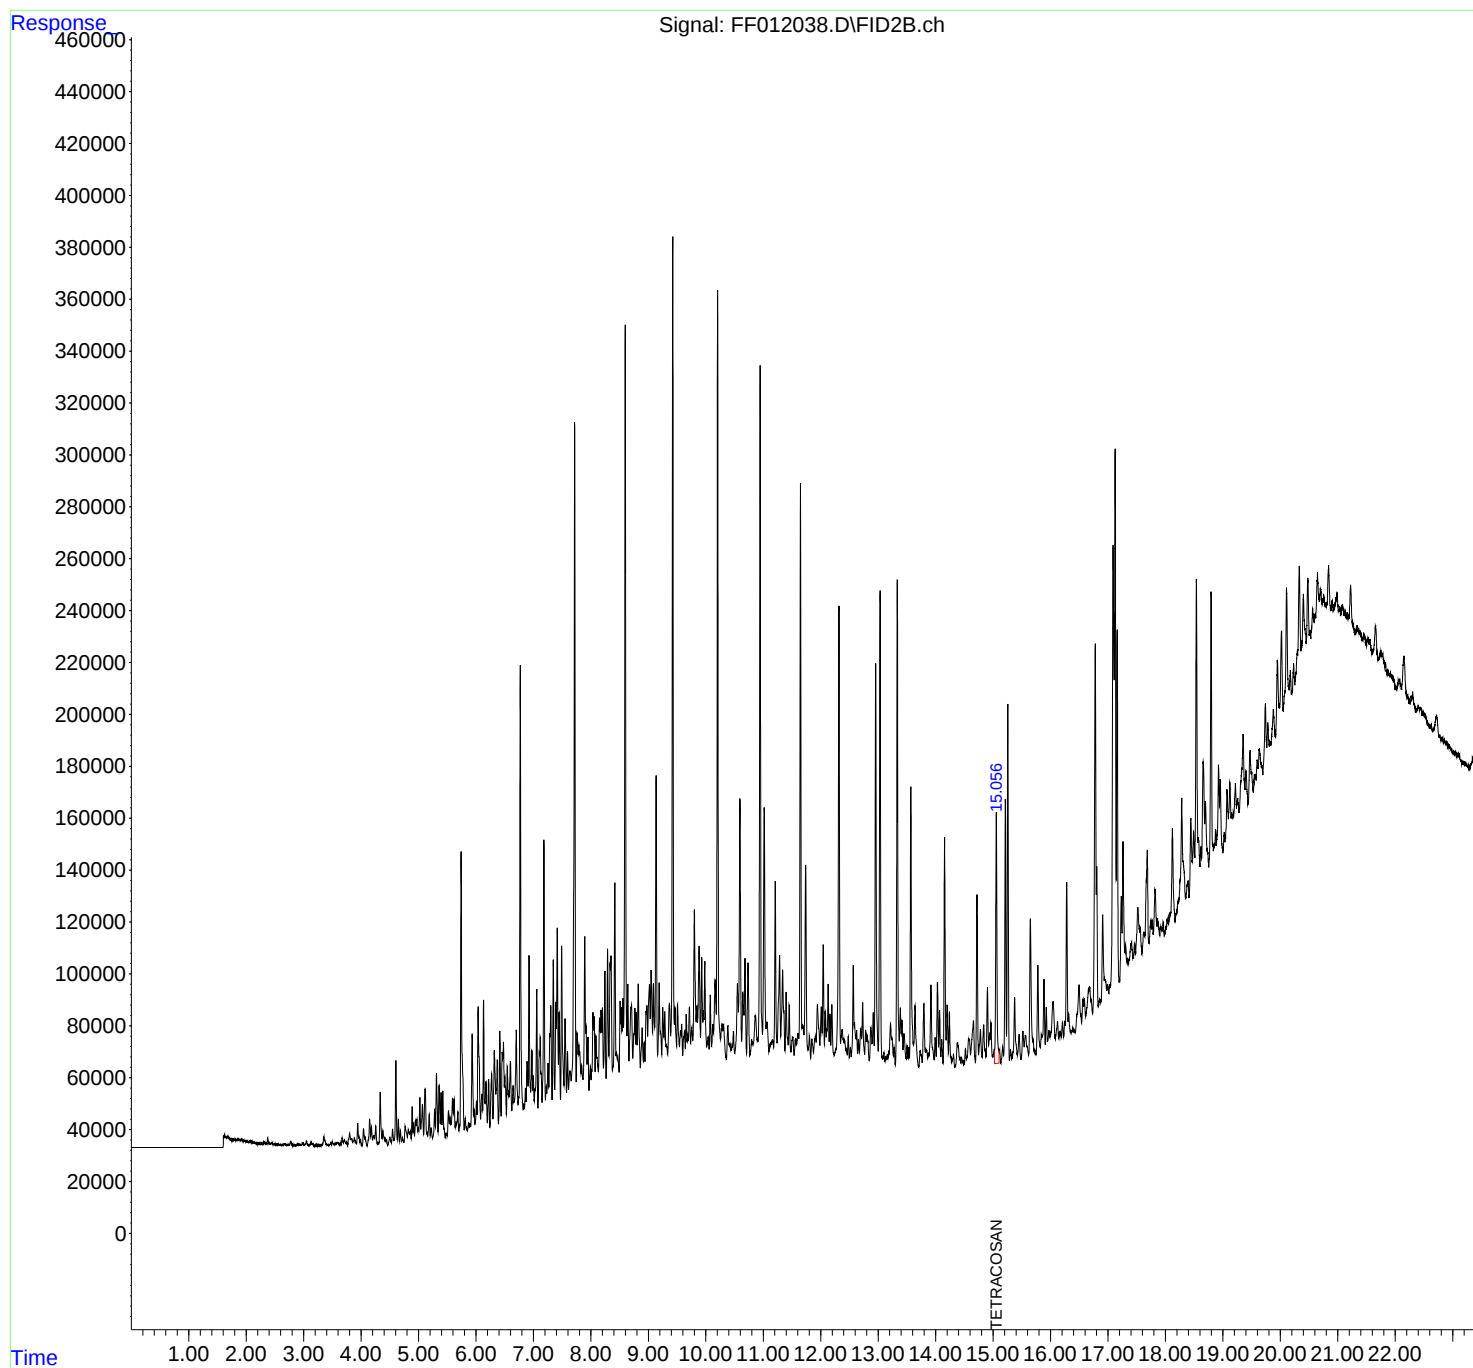

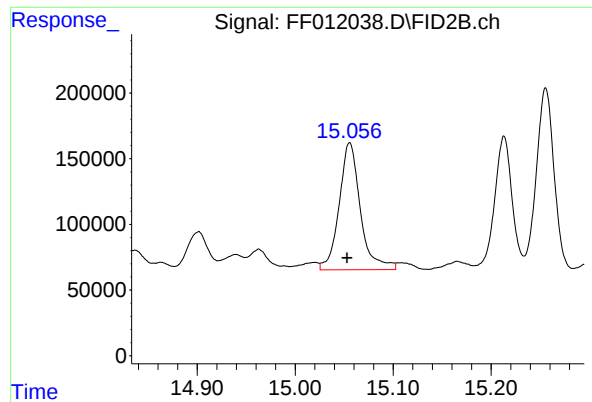

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.056 min
Delta R.T.: 0.003 min
Response: 1455967
Conc: 12.64 ug/ml

Instrument :

FID_F

ClientSampleId :

TWM-TP14-020823