

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
Data File : FF012043.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2023 17:50
Operator : YP\AJ
Sample : 01510-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JPP-59-020823

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

Integration File: autoint1.e
Quant Time: Feb 13 06:27:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	873725	7.582 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021023\
Data File : FF012043.D
Signal(s) : FID2B.ch
Acq On : 10 Feb 2023 17:50
Operator : YP\AJ
Sample : 01510-15
Misc :
ALS Vial : 63 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
JPP-59-020823


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

Integration File: autoint1.e
Quant Time: Feb 13 06:27:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

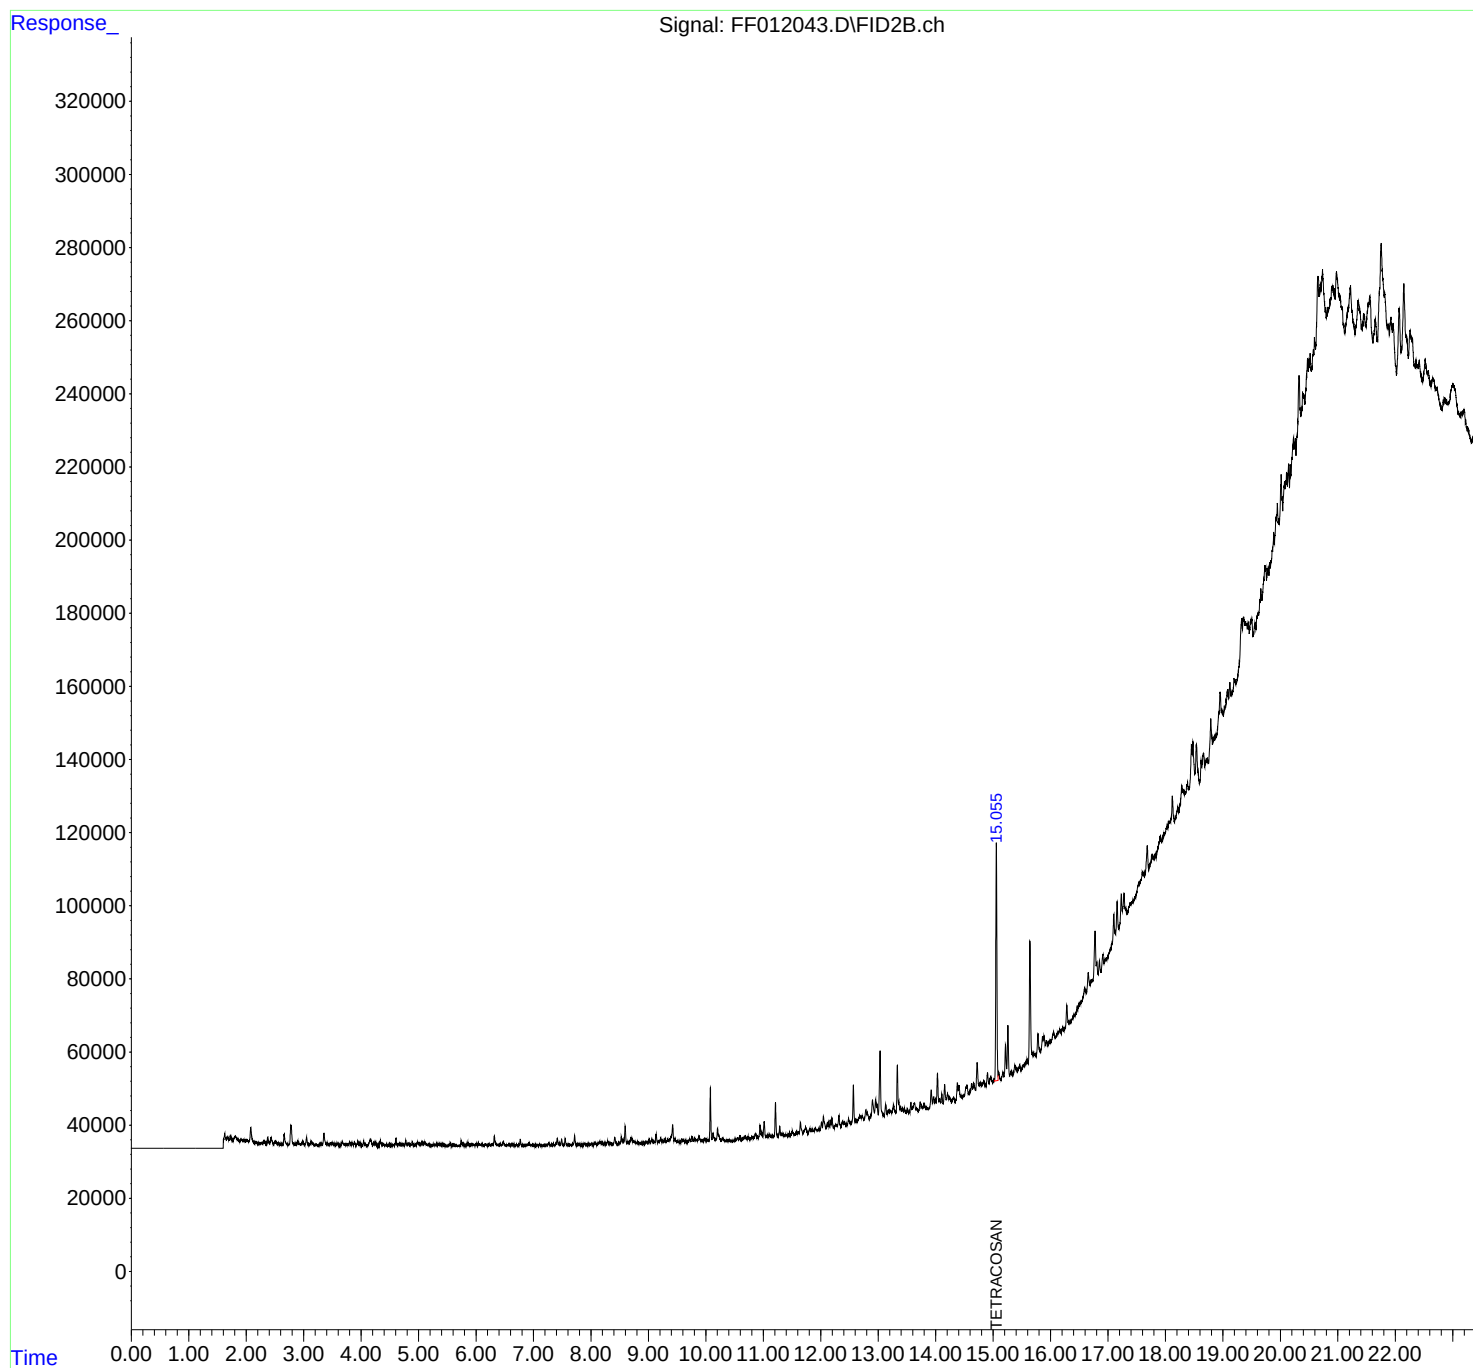

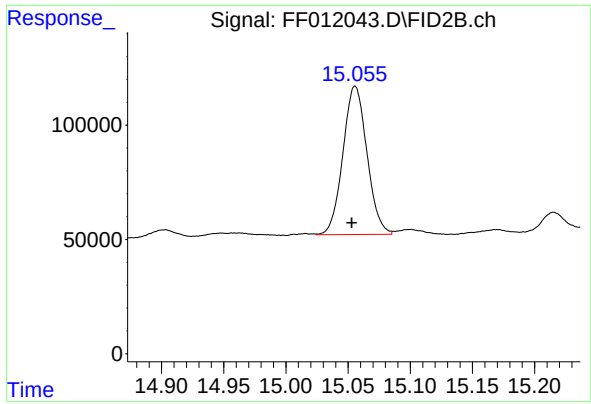

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.055 min
Delta R.T.: 0.002 min
Response: 873725
Conc: 7.58 ug/ml

Instrument :

FID_F

ClientSampleId :

JPP-59-020823

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 02/13/2023

Supervised By :Sohil Jodhani 02/13/2023