

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021120\
 Data File : FF006390.D
 Signal(s) : FID2B.ch
 Acq On : 11 Feb 2020 18:04
 Operator : DD\AJ
 Sample : L1373-01 2X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 12 00:46:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.610	720295	5.912 ug/ml
Target Compounds			
7) N-EICOSANE	12.581f	890372	6.318 ug/ml
8) N-DOCOSANE	13.746	145794	1.037 ug/ml
10) N-TETRACOSANE	14.794	506875	3.627 ug/ml
12) N-OCTACOSANE	16.781	197371	1.430 ug/ml
13) N-TRIACONTANE	17.661	259617	1.877 ug/ml
14) N-DOTRIACONTANE	18.488	384326	2.921 ug/ml
15) N-TETRATRIACONTANE	19.270	72694	0.647 ug/ml
16) N-HEXATRIACONTANE	20.003	316993	3.275 ug/ml
17) N-OCTATRIACONTANE	20.726	153055	2.167 ug/ml
18) N-TETRACONTANE	21.615	417166	5.910 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021120\
Data File : FF006390.D
Signal(s) : FID2B.ch
Acq On : 11 Feb 2020 18:04
Operator : DD\AJ
Sample : L1373-01 2X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 12 00:46:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

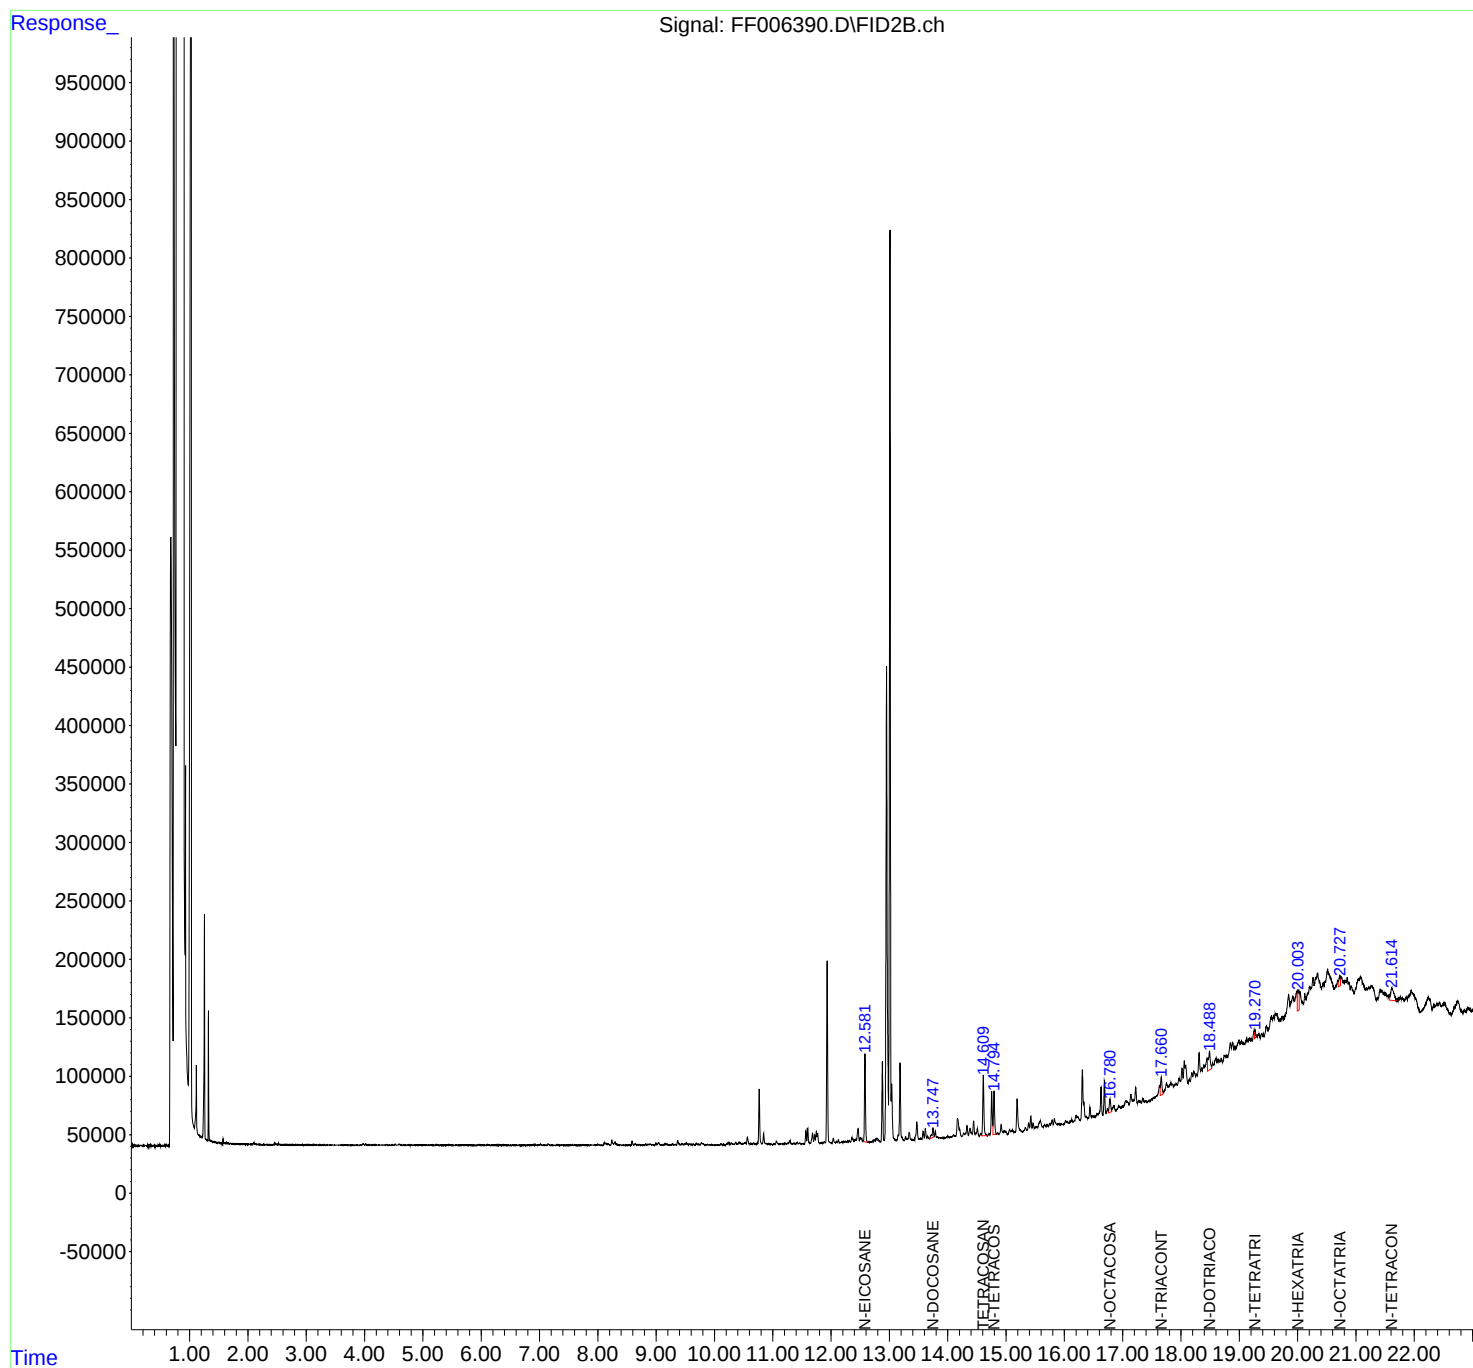

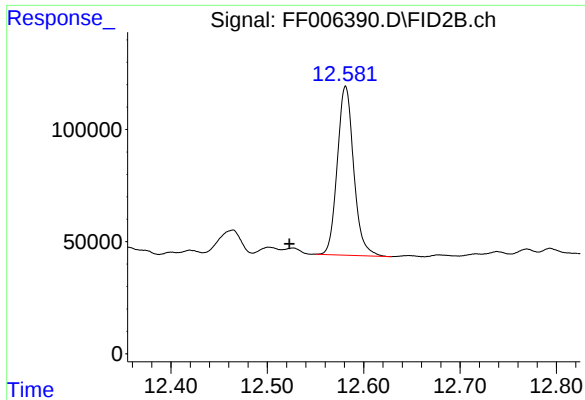


#7 N-EICOSANE

R.T.: 12.581 min
Delta R.T.: 0.058 min
Response: 890372
Conc: 6.32 ug/ml

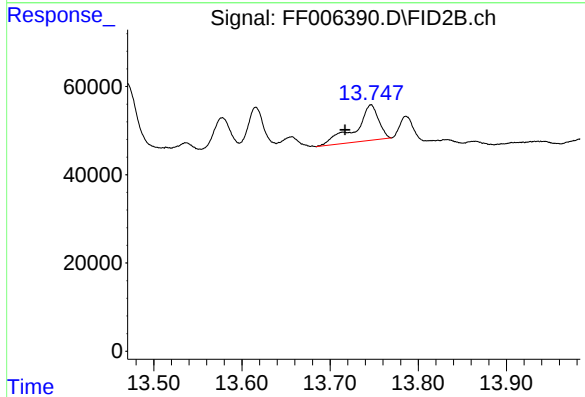


#8 N-DOCOSANE

R.T.: 13.746 min
Delta R.T.: 0.030 min
Response: 145794
Conc: 1.04 ug/ml

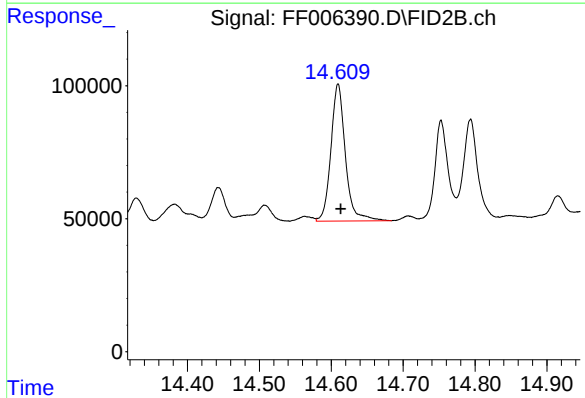


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.610 min
Delta R.T.: -0.004 min
Response: 720295
Conc: 5.91 ug/ml

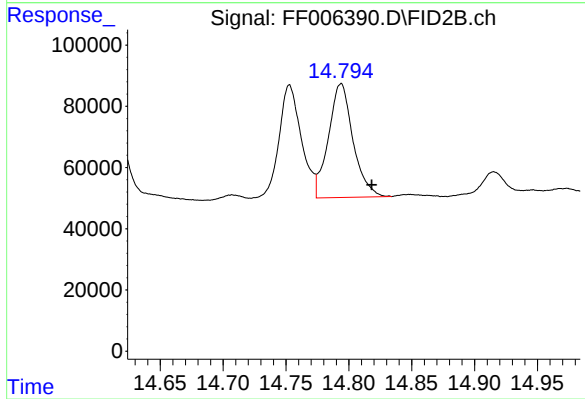


#10 N-TETRACOSANE

R.T.: 14.794 min
Delta R.T.: -0.024 min
Response: 506875
Conc: 3.63 ug/ml

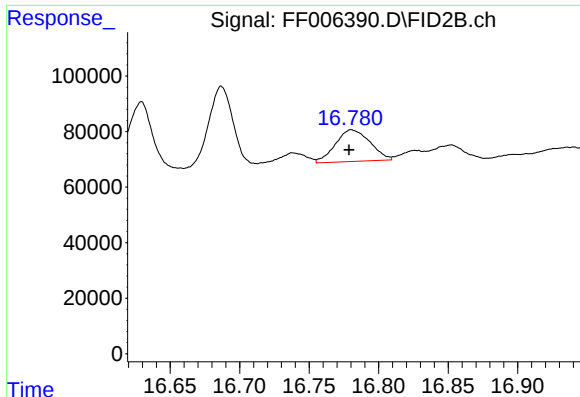


#12 N-OCTACOSANE

R.T.: 16.781 min
Delta R.T.: 0.002 min
Response: 197371
Conc: 1.43 ug/ml

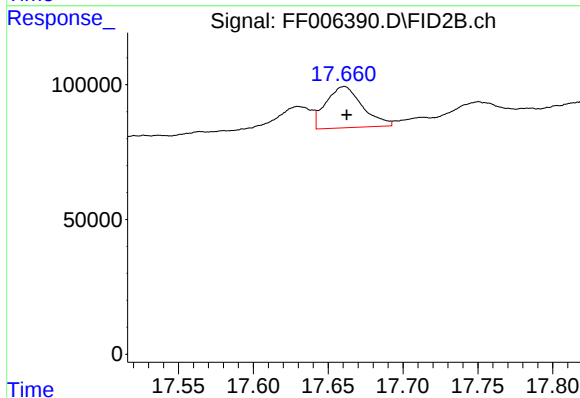


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.002 min
Response: 259617
Conc: 1.88 ug/ml

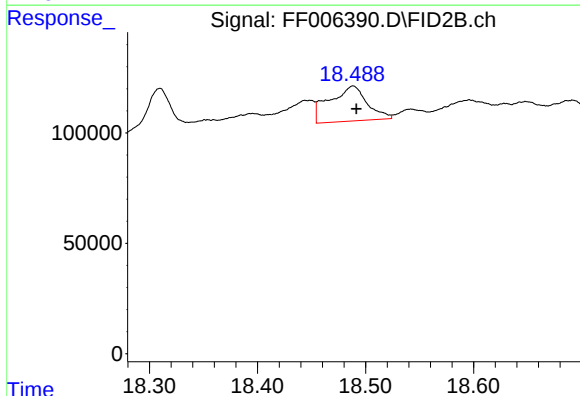


#14 N-DOTRIACONTANE

R.T.: 18.488 min
Delta R.T.: -0.003 min
Response: 384326
Conc: 2.92 ug/ml

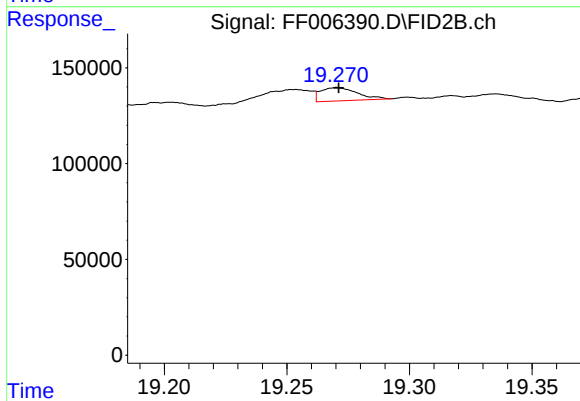


#15 N-TETRATRIACONTANE

R.T.: 19.270 min
Delta R.T.: 0.000 min
Response: 72694
Conc: 0.65 ug/ml

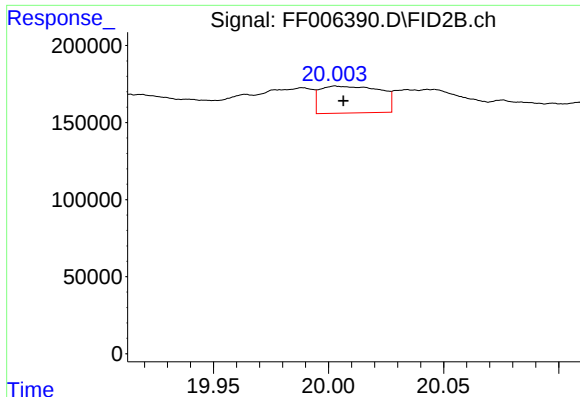


#16 N-HEXATRIACONTANE

R.T.: 20.003 min
Delta R.T.: -0.003 min
Response: 316993
Conc: 3.28 ug/ml

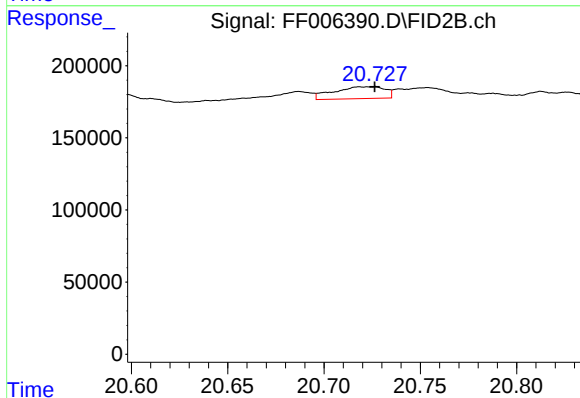

#17 N-OCTATRIACONTANE

R.T.: 20.726 min
Delta R.T.: 0.000 min
Response: 153055
Conc: 2.17 ug/ml

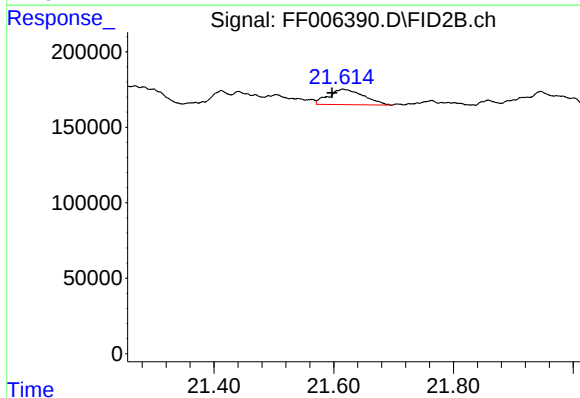

#18 N-TETRACONTANE

R.T.: 21.615 min
Delta R.T.: 0.018 min
Response: 417166
Conc: 5.91 ug/ml