

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021120\
 Data File : FF006392.D
 Signal(s) : FID2B.ch
 Acq On : 11 Feb 2020 19:05
 Operator : DD\AJ
 Sample : L1373-01MS 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 12 00:46:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.610	1477923	12.131 ug/ml
Target Compounds				
2)	N-DECANE	4.374	1368680	10.249 ug/ml
3)	N-DODECANE	6.389	1485176	10.867 ug/ml
4)	N-TETRADECANE	8.180	1532300	11.140 ug/ml
5)	N-HEXADECANE	9.776	1557370	11.100 ug/ml
6)	N-OCTADECANE	11.213	1465531	10.419 ug/ml
7)	N-EICOSANE	12.519	1621039	11.502 ug/mlm
8)	N-DOCOSANE	13.714	1576824	11.220 ug/ml
10)	N-TETRACOSANE	14.799	2639406	18.889 ug/mlm
11)	N-HEXACOSANE	15.831	1423900	10.314 ug/ml
12)	N-OCTACOSANE	16.778	1706725	12.367 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021120\
Data File : FF006392.D
Signal(s) : FID2B.ch
Acq On : 11 Feb 2020 19:05
Operator : DD\AJ
Sample : L1373-01MS 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 12 00:46:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

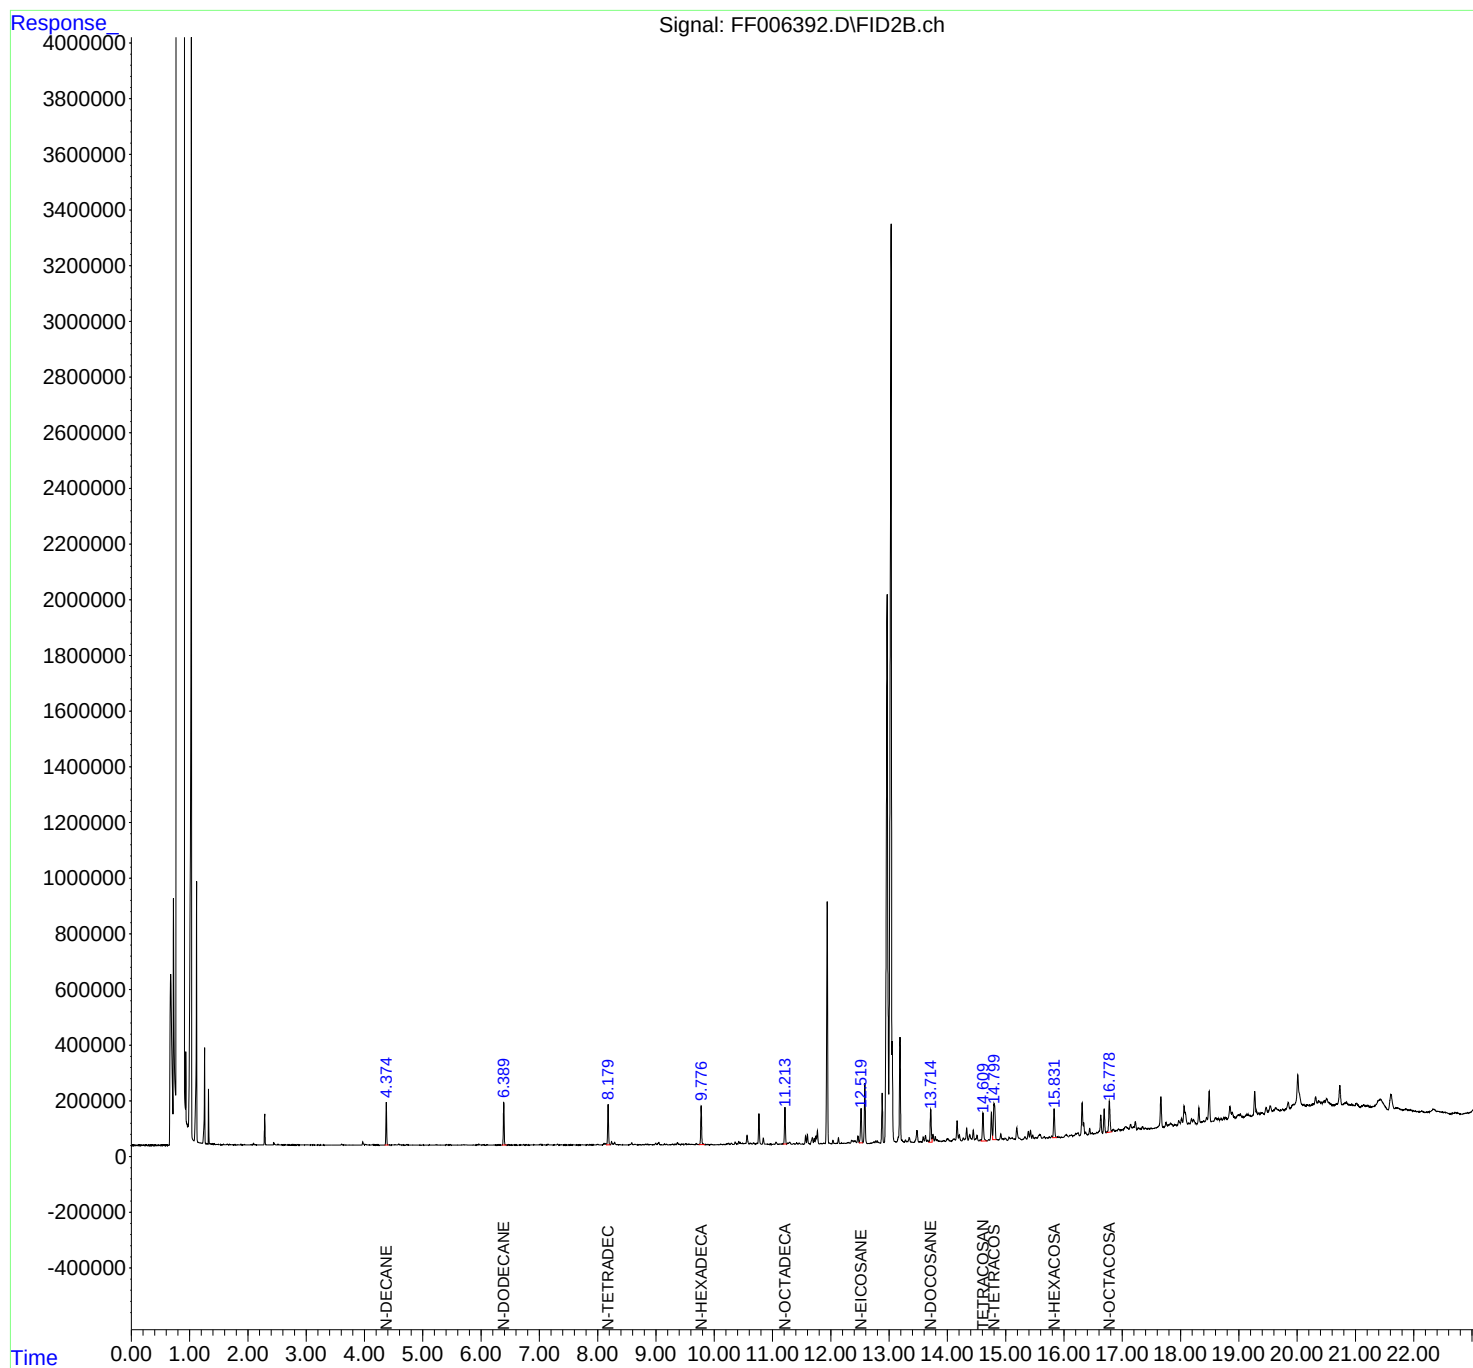

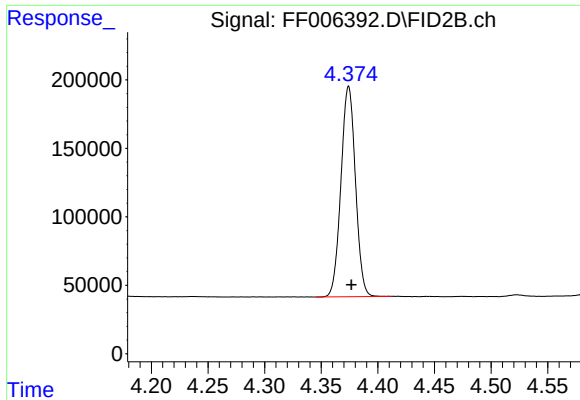


#2 N-DECANE

R.T.: 4.374 min
Delta R.T.: -0.003 min
Response: 1368680
Conc: 10.25 ug/ml

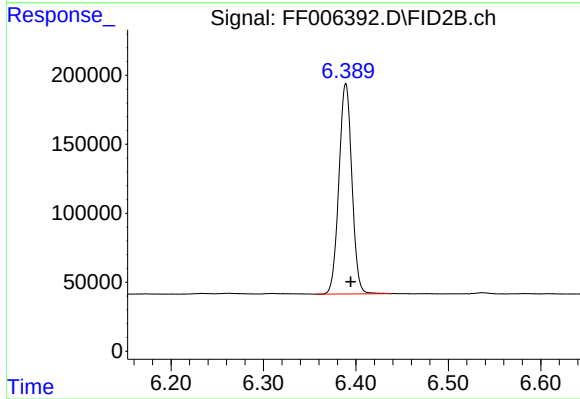


#3 N-DODECANE

R.T.: 6.389 min
Delta R.T.: -0.005 min
Response: 1485176
Conc: 10.87 ug/ml

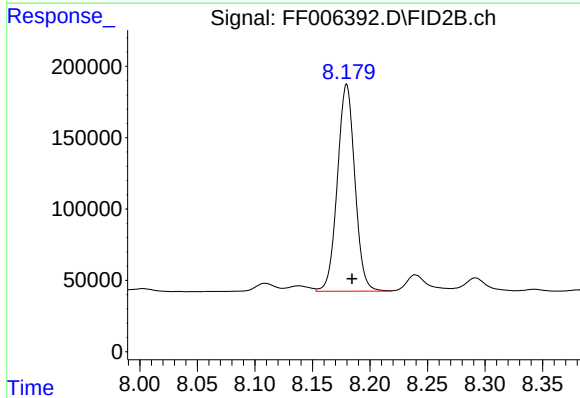


#4 N-TETRADECANE

R.T.: 8.180 min
Delta R.T.: -0.005 min
Response: 1532300
Conc: 11.14 ug/ml

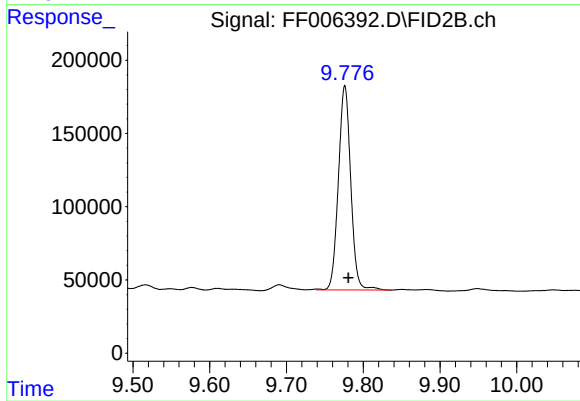


#5 N-HEXADECANE

R.T.: 9.776 min
Delta R.T.: -0.005 min
Response: 1557370
Conc: 11.10 ug/ml

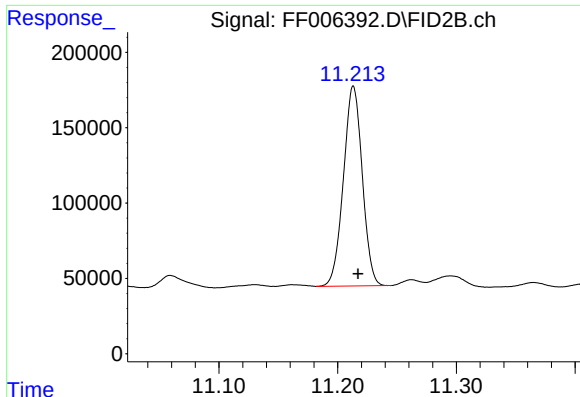


#6 N-OCTADECANE

R.T.: 11.213 min
Delta R.T.: -0.004 min
Response: 1465531
Conc: 10.42 ug/ml

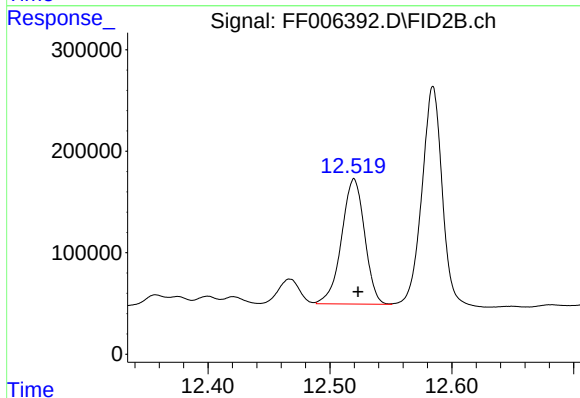


#7 N-EICOSANE

R.T.: 12.519 min
Delta R.T.: -0.004 min
Response: 1621039
Conc: 11.50 ug/ml m

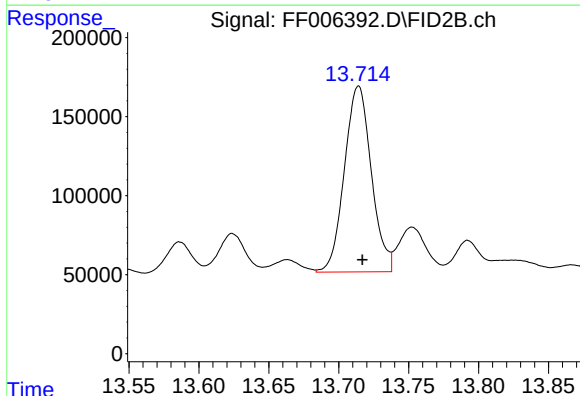


#8 N-DOCOSANE

R.T.: 13.714 min
Delta R.T.: -0.003 min
Response: 1576824
Conc: 11.22 ug/ml

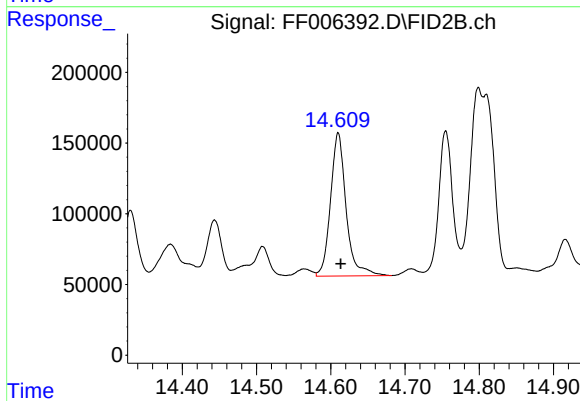


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.610 min
Delta R.T.: -0.003 min
Response: 1477923
Conc: 12.13 ug/ml

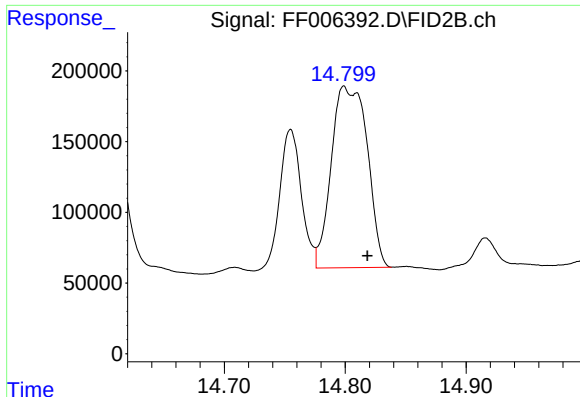


#10 N-TETRACOSANE

R.T.: 14.799 min
Delta R.T.: -0.020 min
Response: 2639406
Conc: 18.89 ug/ml m

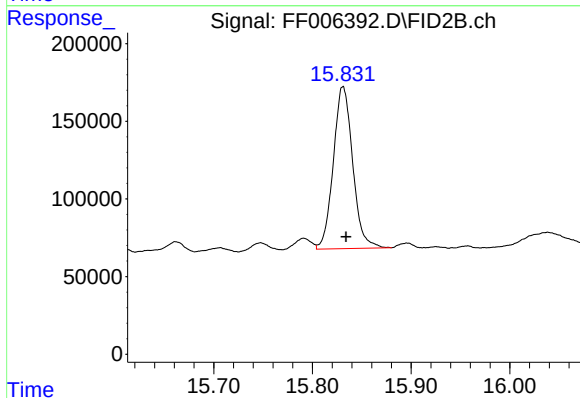

#11 N-HEXACOSANE

R.T.: 15.831 min
Delta R.T.: -0.003 min
Response: 1423900
Conc: 10.31 ug/ml

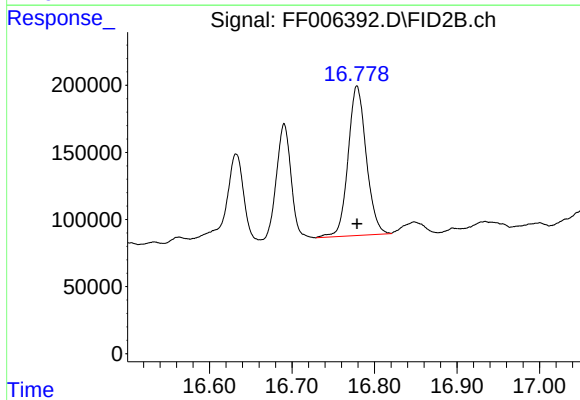

#12 N-OCTACOSANE

R.T.: 16.778 min
Delta R.T.: 0.000 min
Response: 1706725
Conc: 12.37 ug/ml m