

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021219\
 Data File : FF003467.D
 Signal(s) : FID2B.ch
 Acq On : 12 Feb 2019 09:37
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 12 12:22:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	5958451	49.355 ug/ml
Target Compounds			
2) N-DECANE	4.336	7839931	58.581 ug/ml
3) N-DODECANE	6.359	7712632	57.203 ug/ml
4) N-TETRADECANE	8.154	7508645	55.473 ug/ml
5) N-HEXADECANE	9.756	7361639	54.020 ug/ml
6) N-OCTADECANE	11.200	7181878	52.194 ug/ml
7) N-EICOSANE	12.513	6952277	50.556 ug/ml
8) N-DOCOSANE	13.715	6784427	49.587 ug/ml
10) N-TETRACOSANE	14.822	6662378	48.990 ug/ml
11) N-HEXACOSANE	15.846	6627659	48.864 ug/ml
12) N-OCTACOSANE	16.801	6682089	48.805 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021219\
Data File : FF003467.D
Signal(s) : FID2B.ch
Acq On : 12 Feb 2019 09:37
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 12 12:22:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

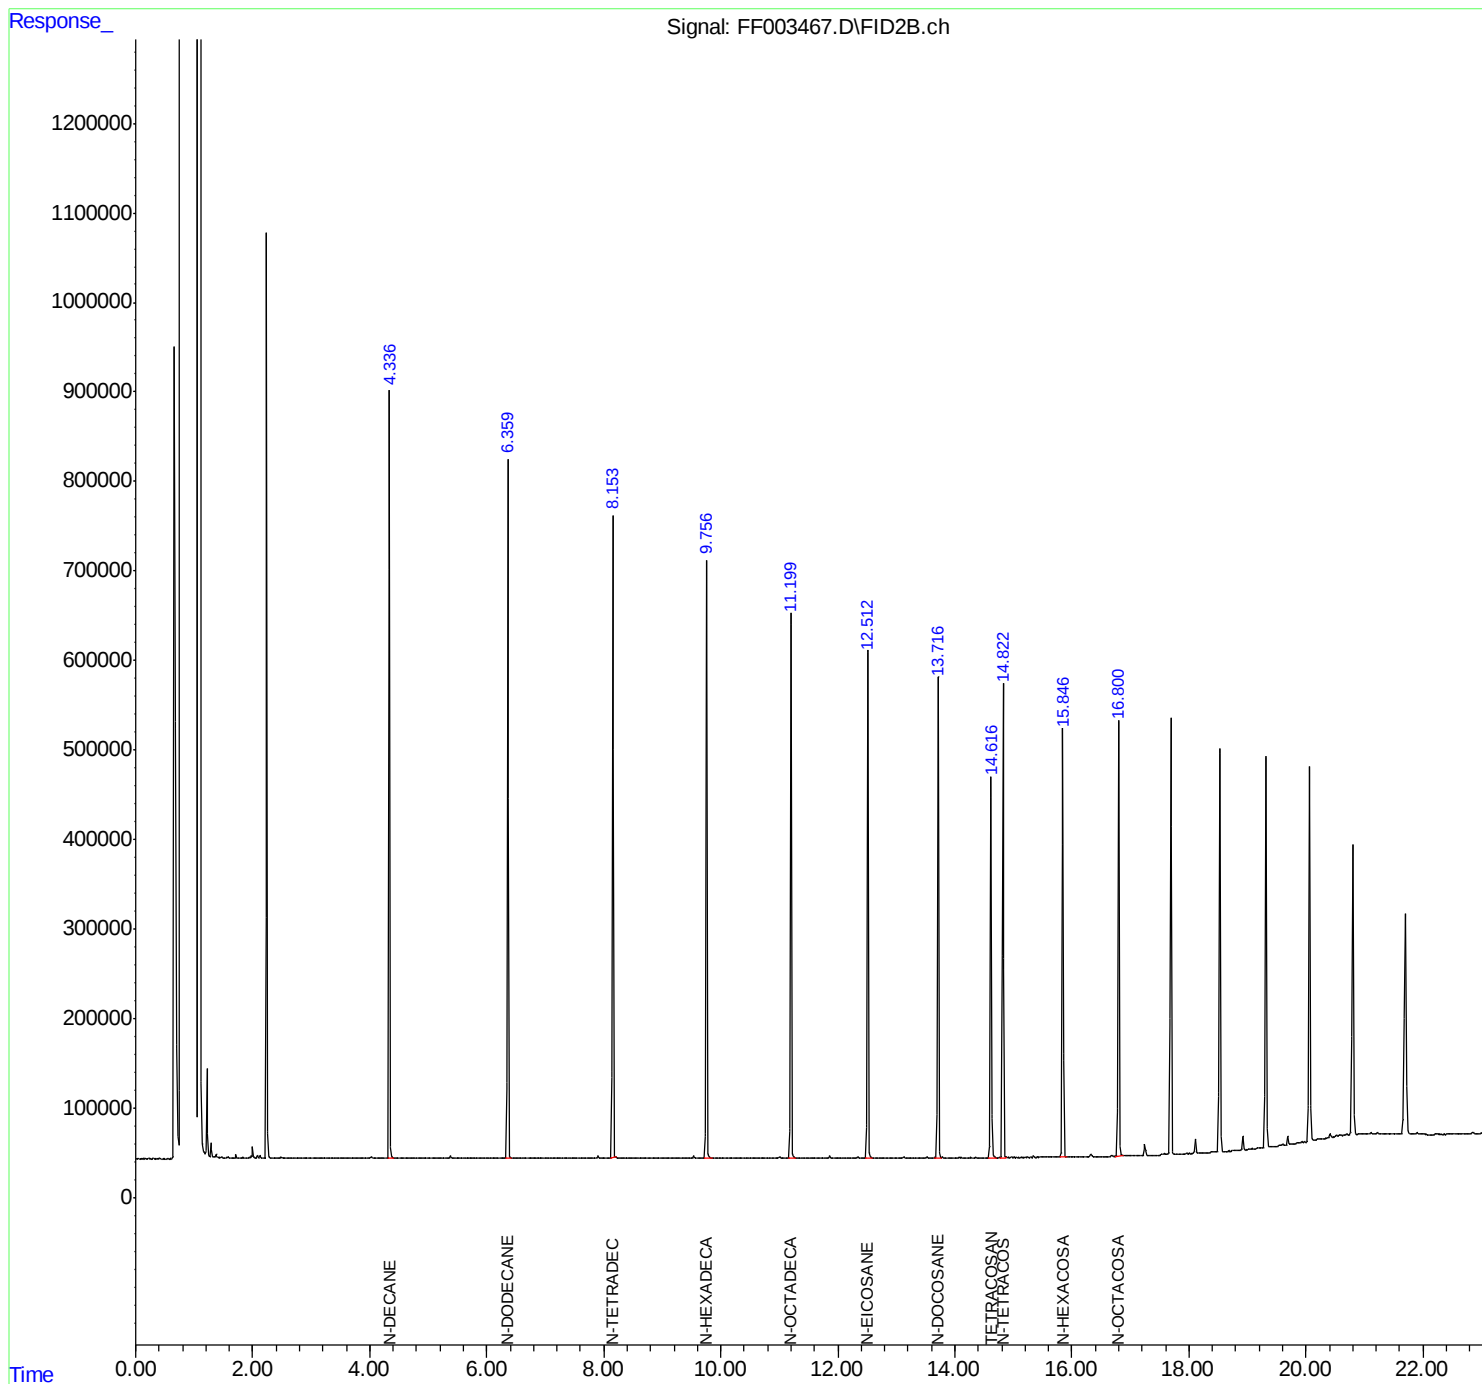

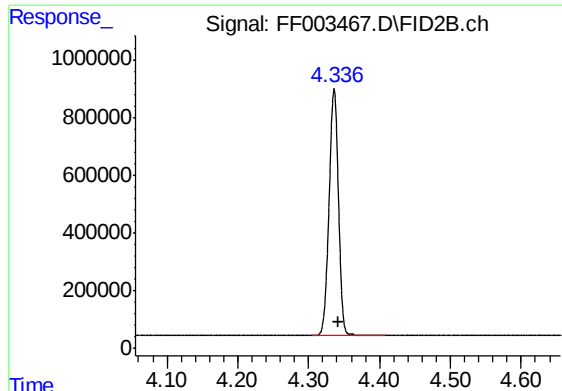


#2 N-DECANE

R.T.: 4.336 min
Delta R.T.: -0.006 min
Response: 7839931
Conc: 58.58 ug/ml

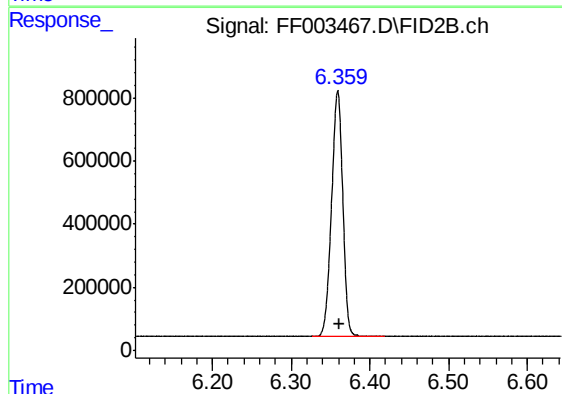


#3 N-DODECANE

R.T.: 6.359 min
Delta R.T.: -0.002 min
Response: 7712632
Conc: 57.20 ug/ml

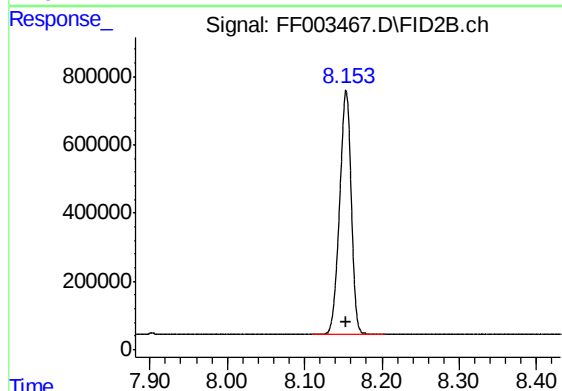


#4 N-TETRADECANE

R.T.: 8.154 min
Delta R.T.: 0.000 min
Response: 7508645
Conc: 55.47 ug/ml

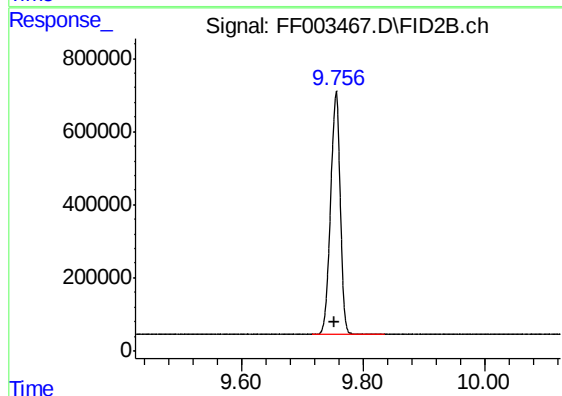


#5 N-HEXADECANE

R.T.: 9.756 min
Delta R.T.: 0.004 min
Response: 7361639
Conc: 54.02 ug/ml

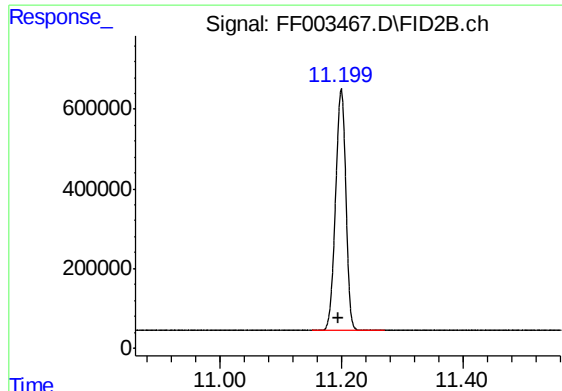


#6 N-OCTADECANE

R.T.: 11.200 min
Delta R.T.: 0.004 min
Response: 7181878
Conc: 52.19 ug/ml

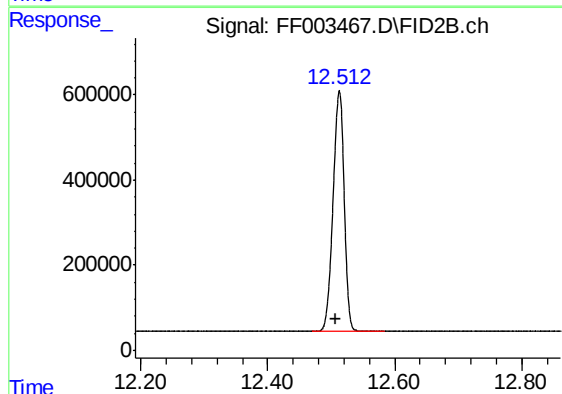


#7 N-EICOSANE

R.T.: 12.513 min
Delta R.T.: 0.005 min
Response: 6952277
Conc: 50.56 ug/ml

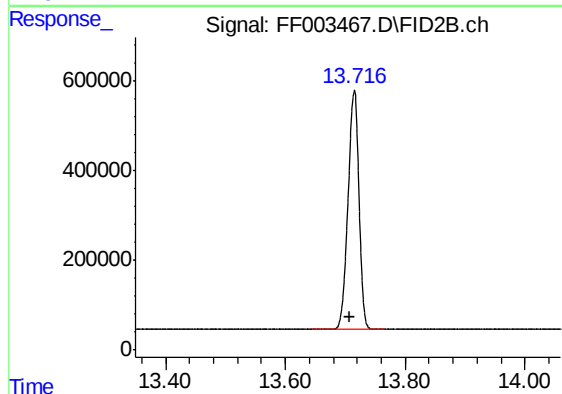


#8 N-DOCOSANE

R.T.: 13.715 min
Delta R.T.: 0.007 min
Response: 6784427
Conc: 49.59 ug/ml

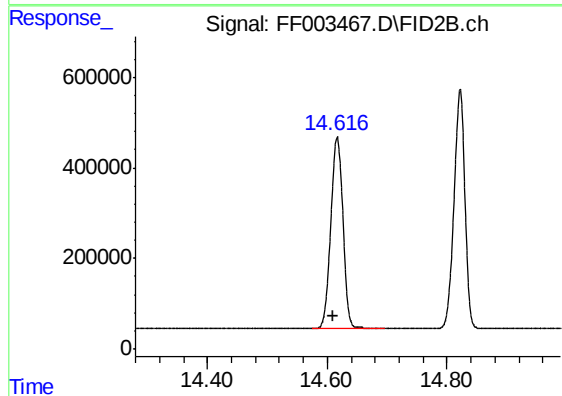


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min
Delta R.T.: 0.006 min
Response: 5958451
Conc: 49.35 ug/ml

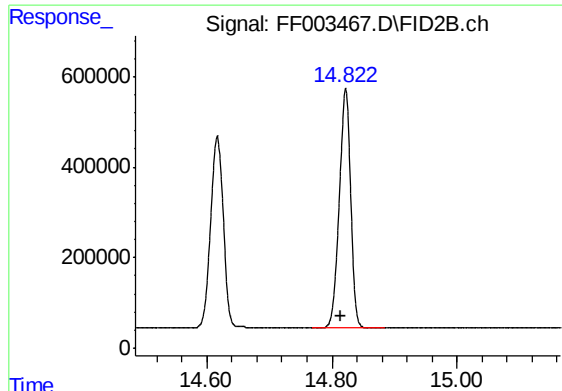


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: 0.008 min
Response: 6662378
Conc: 48.99 ug/ml

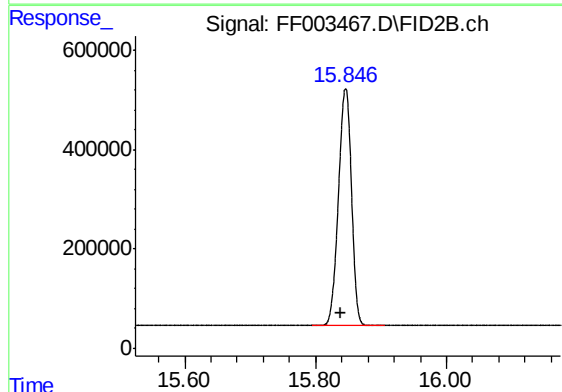

#11 N-HEXACOSANE

R.T.: 15.846 min
Delta R.T.: 0.008 min
Response: 6627659
Conc: 48.86 ug/ml

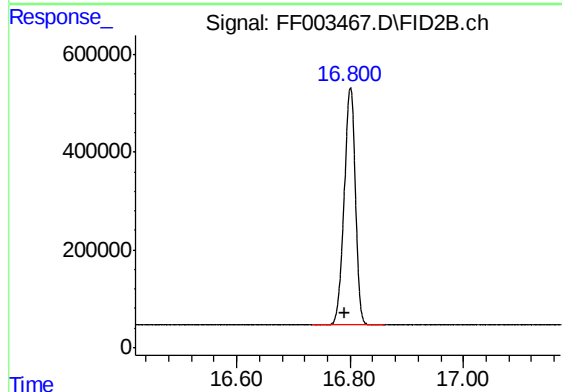

#12 N-OCTACOSANE

R.T.: 16.801 min
Delta R.T.: 0.009 min
Response: 6682089
Conc: 48.80 ug/ml