

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021219\
 Data File : FF003471.D
 Signal(s) : FID2B.ch
 Acq On : 12 Feb 2019 12:46
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 12 13:38:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.618	5856931	48.514 ug/ml
Target Compounds			
2) N-DECANE	4.342	7767555	58.040 ug/ml
3) N-DODECANE	6.364	7630448	56.594 ug/ml
4) N-TETRADECANE	8.157	7415079	54.782 ug/ml
5) N-HEXADECANE	9.759	7244060	53.157 ug/ml
6) N-OCTADECANE	11.202	7055155	51.273 ug/ml
7) N-EICOSANE	12.514	6826477	49.642 ug/ml
8) N-DOCOSANE	13.717	6657463	48.659 ug/ml
10) N-TETRACOSANE	14.822	6544078	48.120 ug/ml
11) N-HEXACOSANE	15.845	6528373	48.132 ug/ml
12) N-OCTACOSANE	16.800	6601198	48.214 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021219\
Data File : FF003471.D
Signal(s) : FID2B.ch
Acq On : 12 Feb 2019 12:46
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 12 13:38:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

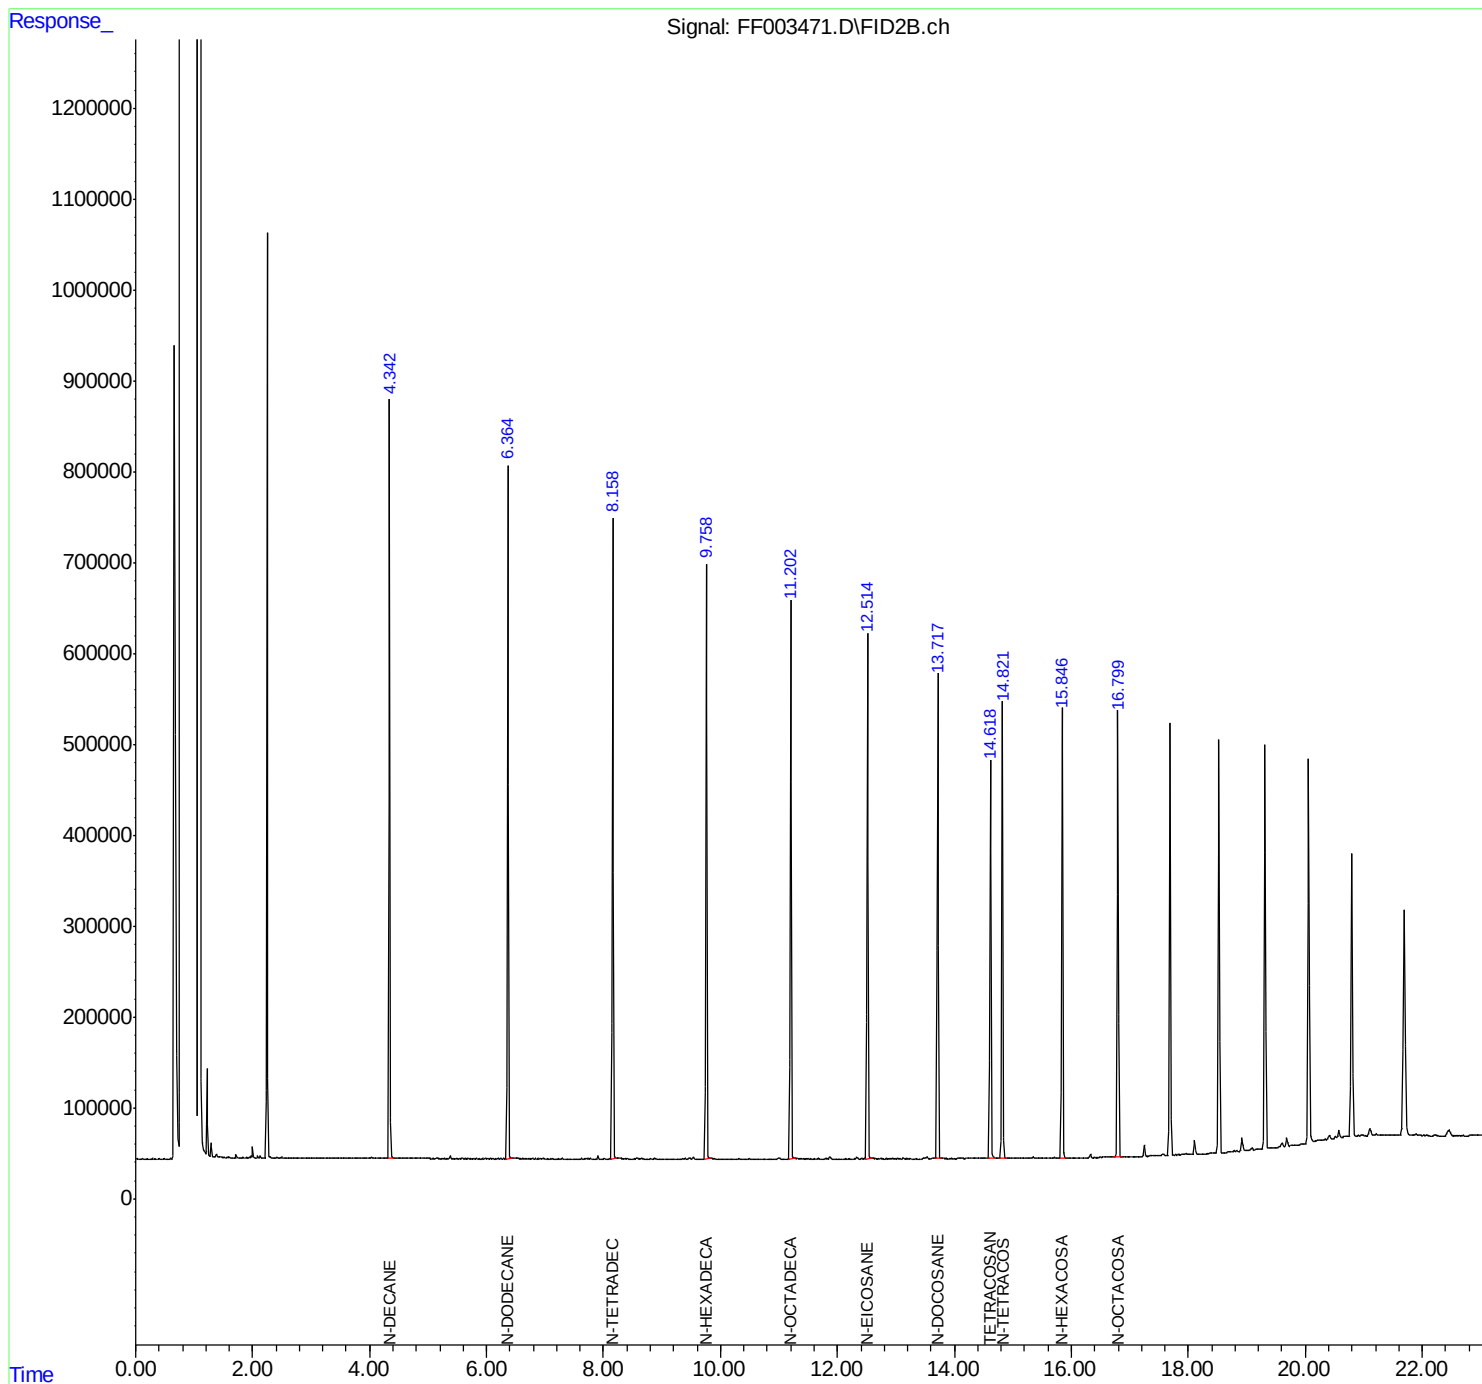

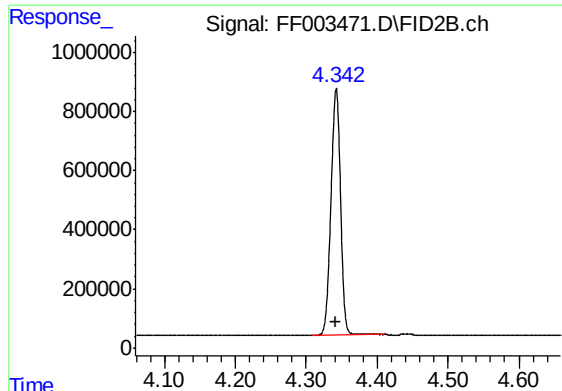


#2 N-DECANE

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 7767555
Conc: 58.04 ug/ml

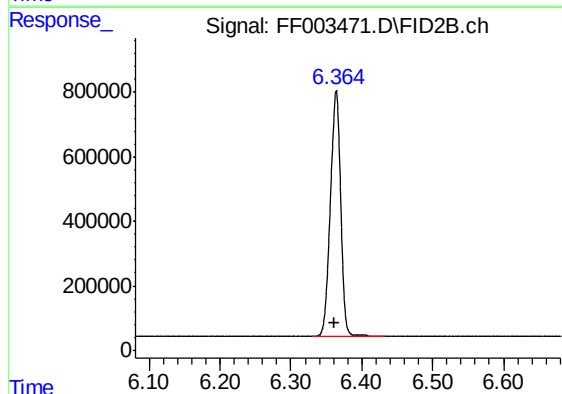


#3 N-DODECANE

R.T.: 6.364 min
Delta R.T.: 0.003 min
Response: 7630448
Conc: 56.59 ug/ml

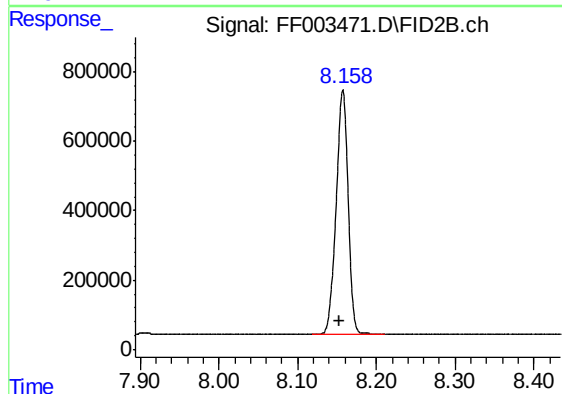


#4 N-TETRADECANE

R.T.: 8.157 min
Delta R.T.: 0.004 min
Response: 7415079
Conc: 54.78 ug/ml

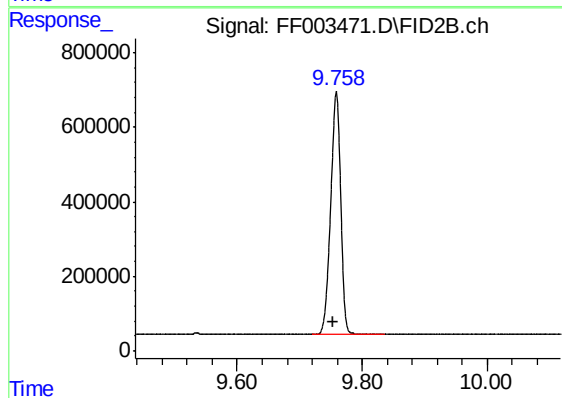


#5 N-HEXADECANE

R.T.: 9.759 min
Delta R.T.: 0.006 min
Response: 7244060
Conc: 53.16 ug/ml

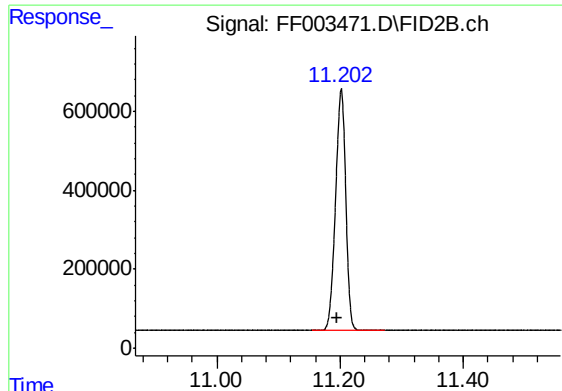


#6 N-OCTADECANE

R.T.: 11.202 min
Delta R.T.: 0.007 min
Response: 7055155
Conc: 51.27 ug/ml

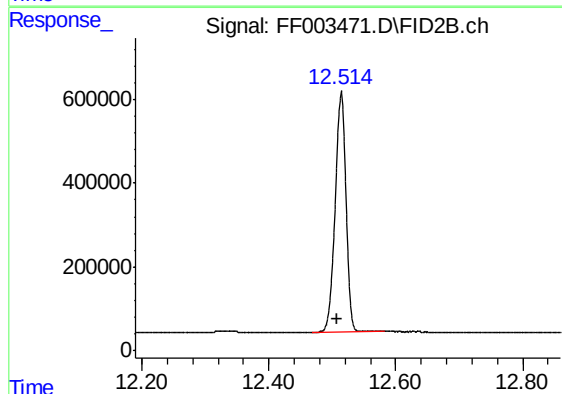


#7 N-EICOSANE

R.T.: 12.514 min
Delta R.T.: 0.006 min
Response: 6826477
Conc: 49.64 ug/ml

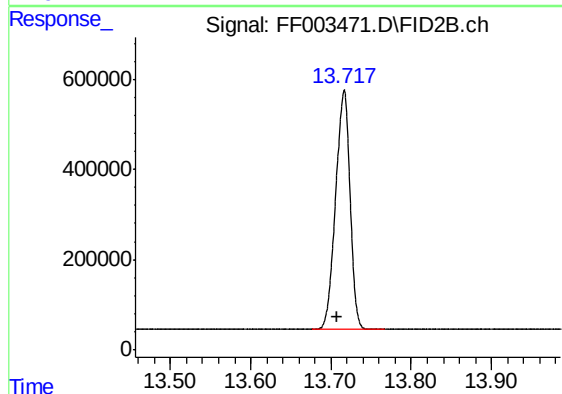


#8 N-DOCOSANE

R.T.: 13.717 min
Delta R.T.: 0.009 min
Response: 6657463
Conc: 48.66 ug/ml

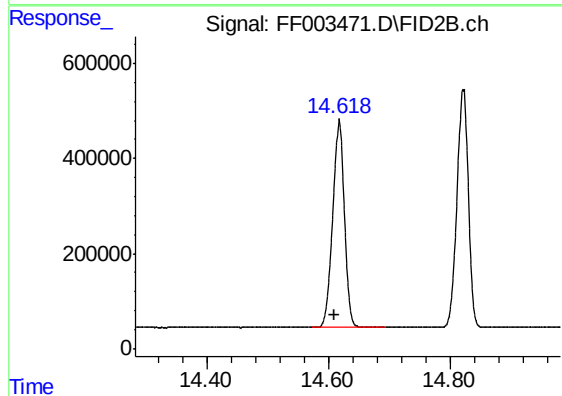


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.618 min
Delta R.T.: 0.008 min
Response: 5856931
Conc: 48.51 ug/ml

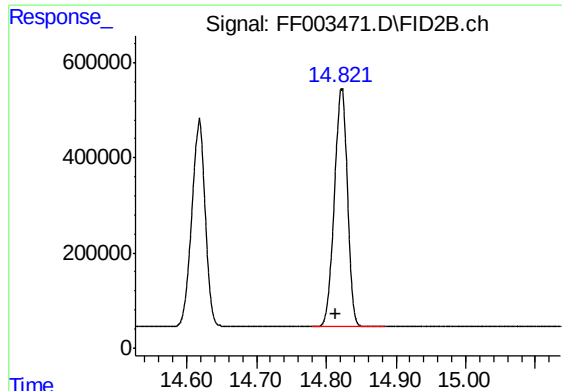


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: 0.008 min
Response: 6544078
Conc: 48.12 ug/ml

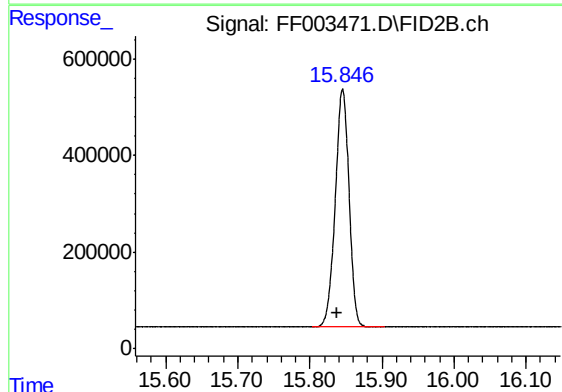

#11 N-HEXACOSANE

R.T.: 15.845 min
Delta R.T.: 0.007 min
Response: 6528373
Conc: 48.13 ug/ml

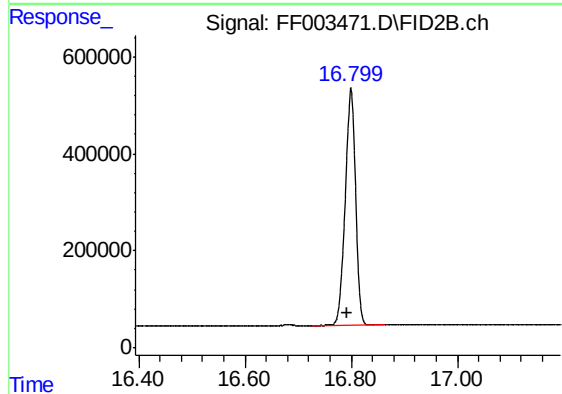

#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.008 min
Response: 6601198
Conc: 48.21 ug/ml