

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
Data File : FF012046.D
Signal(s) : FID2B.ch
Acq On : 13 Feb 2023 09:10
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 01:31:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.950	109413	0.841 ug/ml
15) N-TETRATRIACONTANE	19.733	97189	0.873 ug/ml
16) N-HEXATRIACONTANE	20.458	96806	0.942 ug/ml
17) N-OCTATRIACONTANE	21.210	75132	0.763 ug/ml
18) N-TETRACONTANE	22.165	178347	1.721 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
Data File : FF012046.D
Signal(s) : FID2B.ch
Acq On : 13 Feb 2023 09:10
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 01:31:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

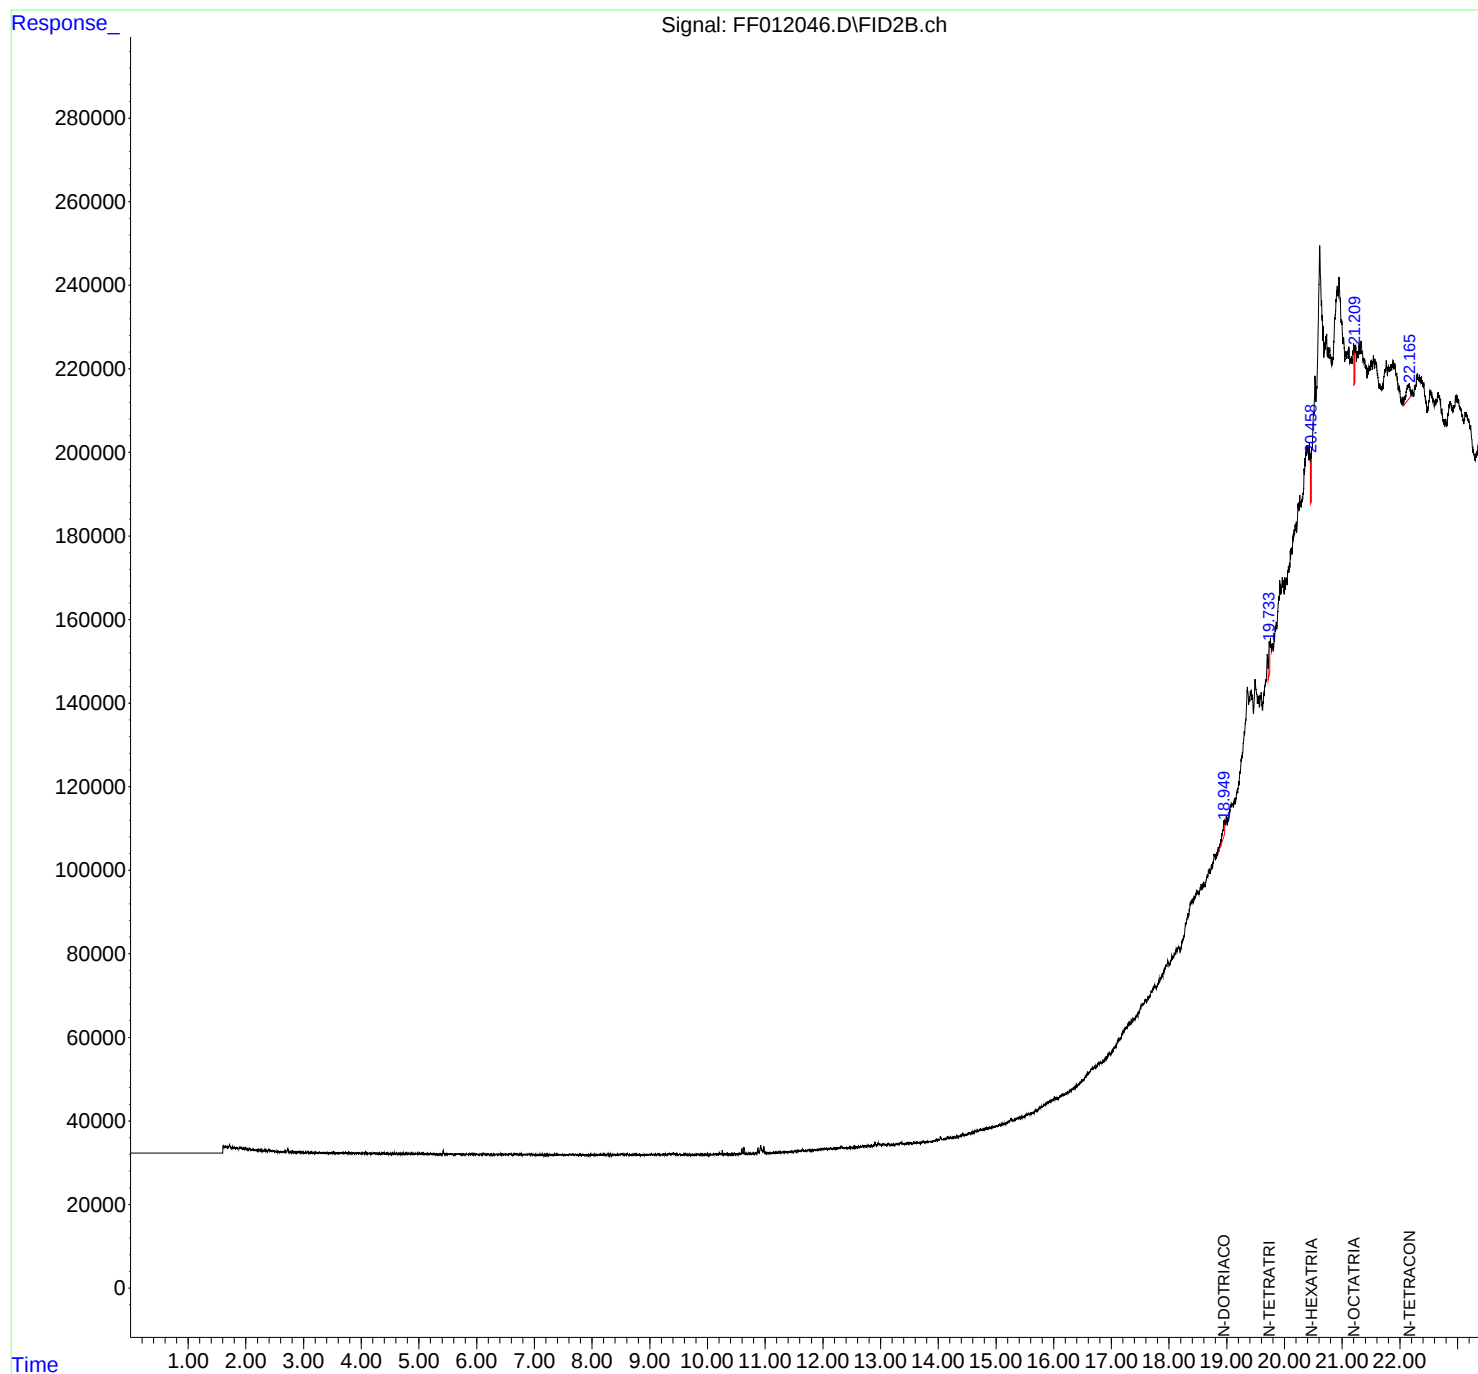


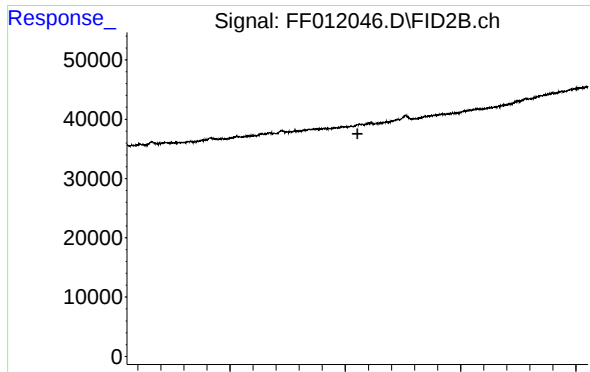

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

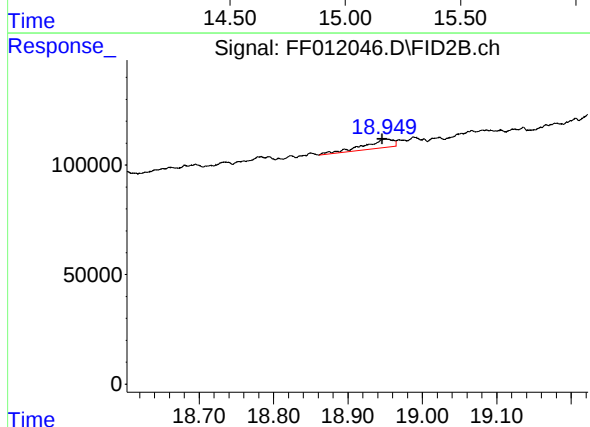


#14 N-DOTRIACONTANE

R.T.: 18.950 min
Delta R.T.: 0.004 min
Response: 109413
Conc: 0.84 ug/ml

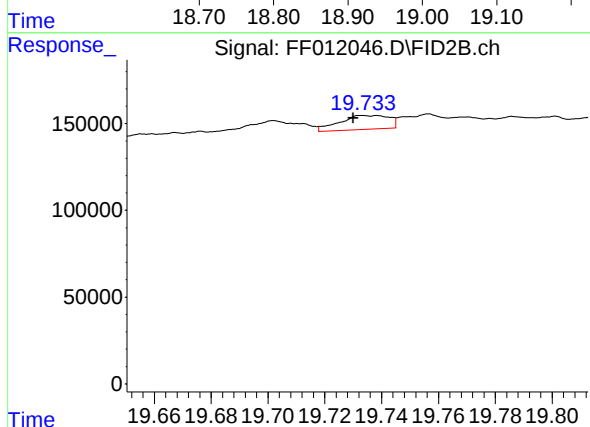


#15 N-TETRATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.003 min
Response: 97189
Conc: 0.87 ug/ml

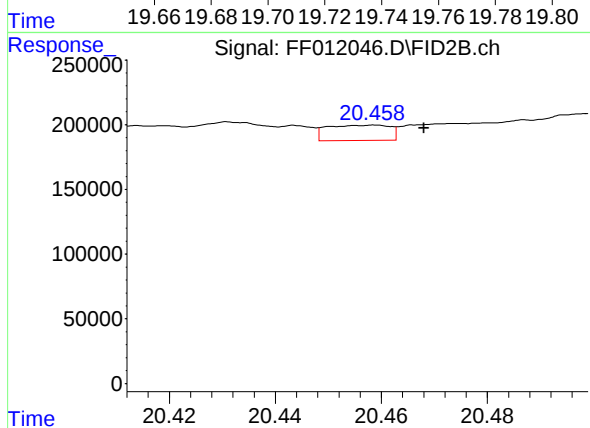

#16 N-HEXATRIACONTANE


R.T.: 20.458 min
Delta R.T.: -0.010 min
Response: 96806
Conc: 0.94 ug/ml

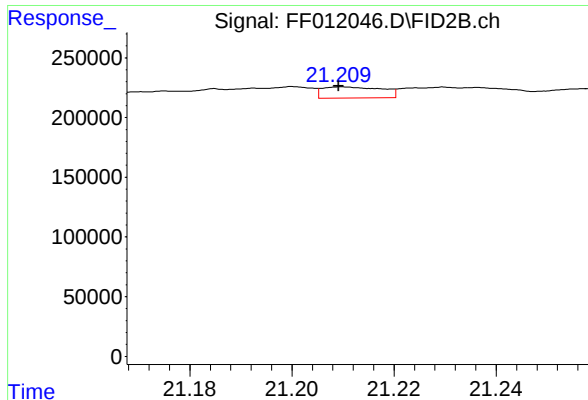

#17 N-OCTATRIACONTANE

R.T.: 21.210 min
Delta R.T.: 0.000 min
Response: 75132
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

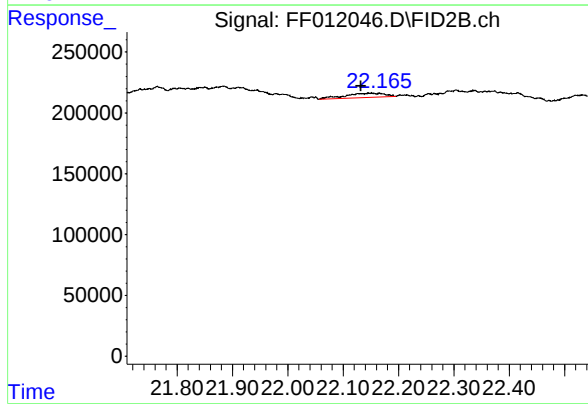

#18 N-TETRACONTANE

R.T.: 22.165 min
Delta R.T.: 0.033 min
Response: 178347
Conc: 1.72 ug/ml