

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
 Data File : FF012049.D
 Signal(s) : FID2B.ch
 Acq On : 13 Feb 2023 10:57
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 01:32:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.763	2404668	20.074 ug/ml
12) N-OCTACOSANE	17.236	2500050	19.226 ug/ml
13) N-TRIACONTANE	18.122	72530	0.562 ug/ml
14) N-DOTRIACONTANE	18.956	245766	1.888 ug/ml
15) N-TETRATRIACONTANE	19.742	189283	1.700 ug/ml
16) N-HEXATRIACONTANE	20.486	122901	1.196 ug/ml
17) N-OCTATRIACONTANE	21.228	57118	0.580 ug/ml
18) N-TETRACONTANE	22.156	144037	1.390 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
Data File : FF012049.D
Signal(s) : FID2B.ch
Acq On : 13 Feb 2023 10:57
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 01:32:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

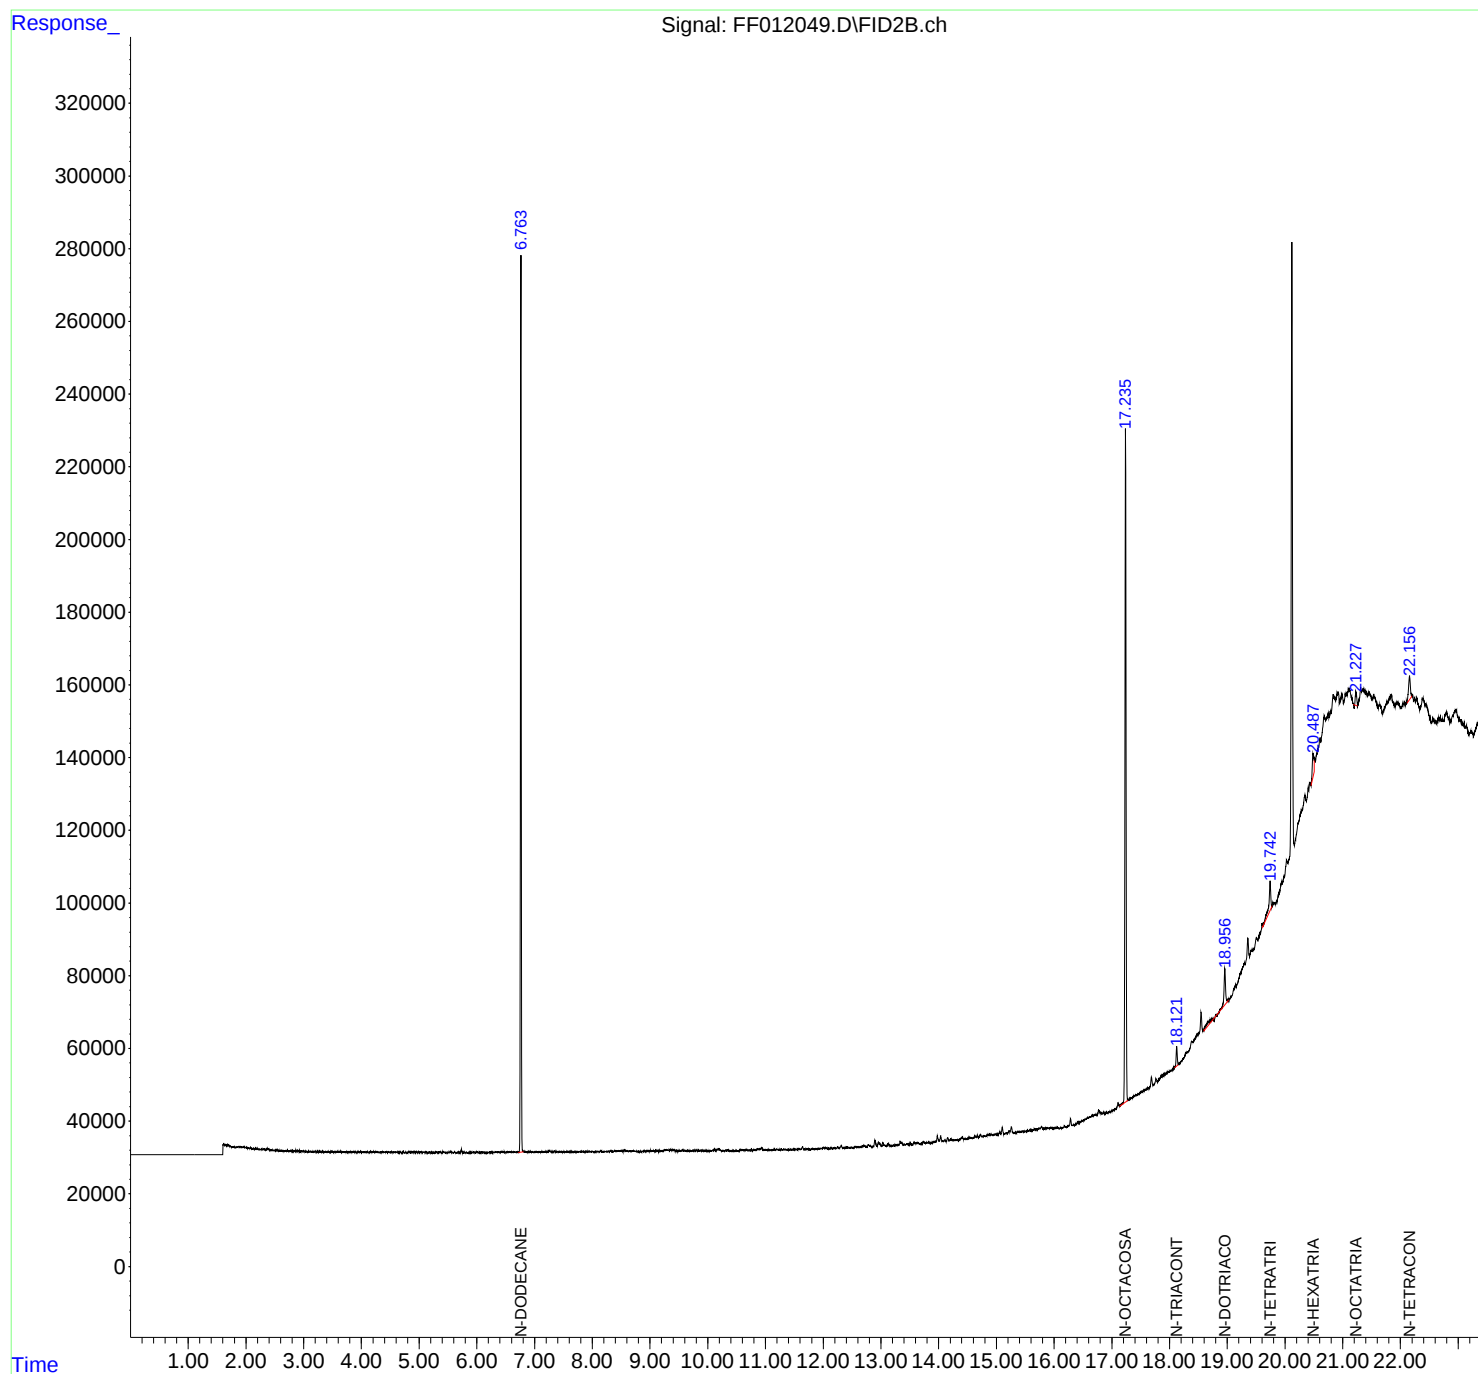


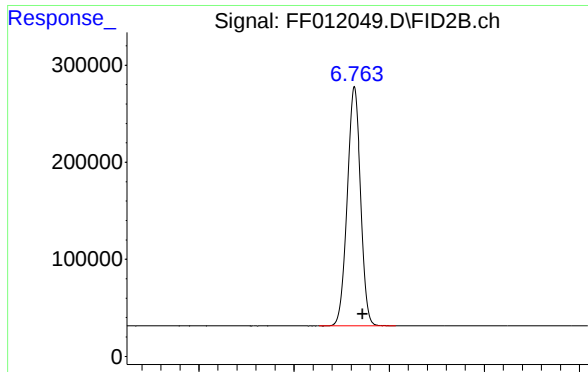

#3 N-DODECANE


R.T.: 6.763 min
Delta R.T.: -0.009 min
Response: 2404668
Conc: 20.07 ug/ml

Instrument :
FID_F
ClientSampleId :

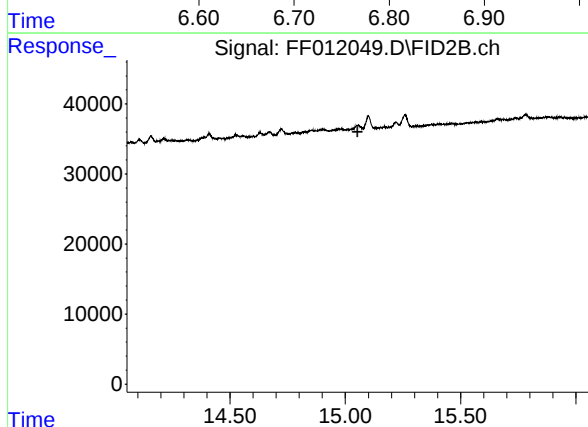


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

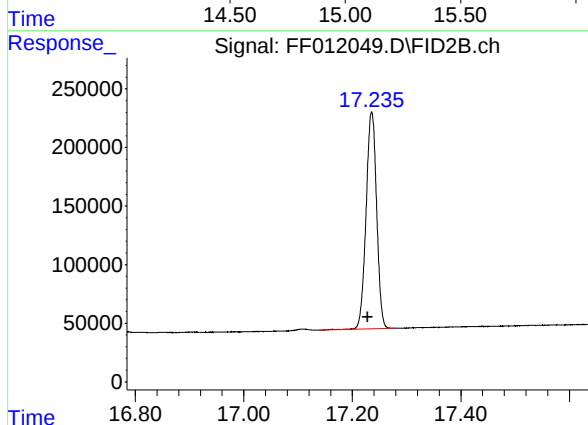


#12 N-OCTACOSANE

R.T.: 17.236 min
Delta R.T.: 0.007 min
Response: 2500050
Conc: 19.23 ug/ml

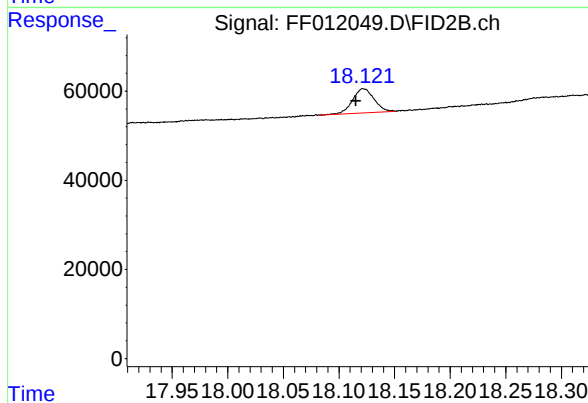

#13 N-TRIACONTANE


R.T.: 18.122 min
Delta R.T.: 0.007 min
Response: 72530
Conc: 0.56 ug/ml

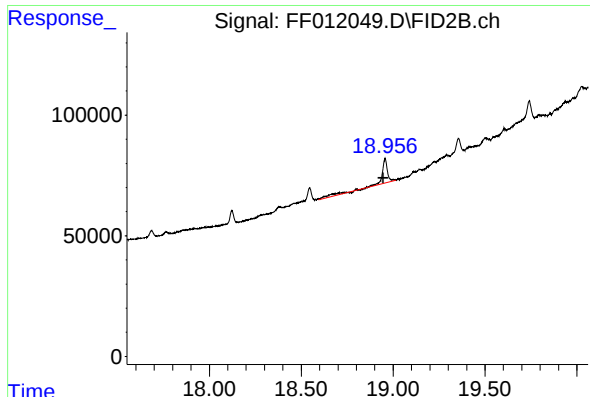

#14 N-DOTRIACONTANE


R.T.: 18.956 min
Delta R.T.: 0.010 min
Response: 245766
Conc: 1.89 ug/ml

Instrument :
FID_F
ClientSampleId :

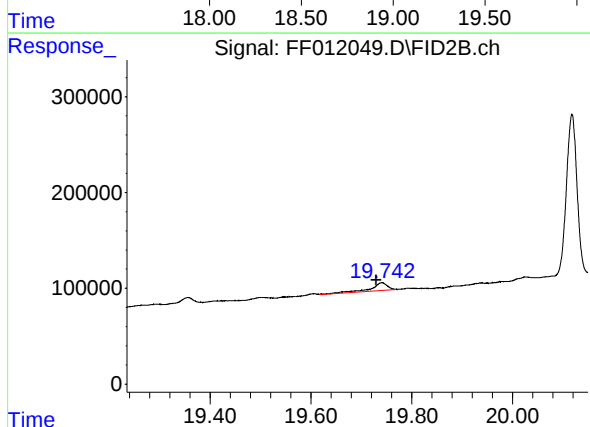


#15 N-TETRATRIACONTANE

R.T.: 19.742 min
Delta R.T.: 0.011 min
Response: 189283
Conc: 1.70 ug/ml

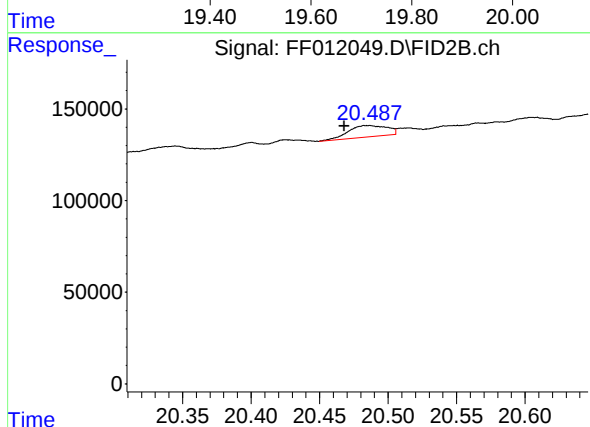


#16 N-HEXATRIACONTANE

R.T.: 20.486 min
Delta R.T.: 0.018 min
Response: 122901
Conc: 1.20 ug/ml

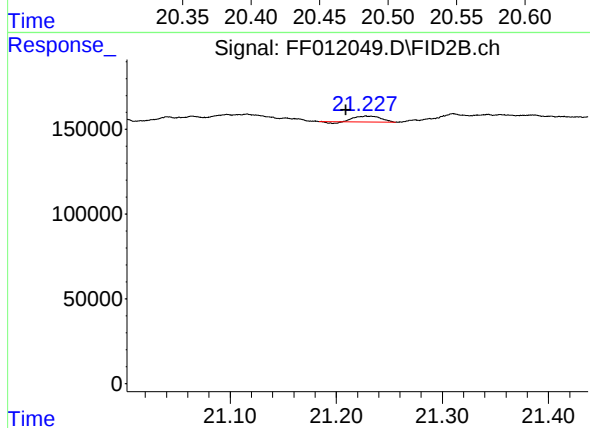

#17 N-OCTATRIACONTANE

R.T.: 21.228 min
Delta R.T.: 0.019 min
Response: 57118
Conc: 0.58 ug/ml

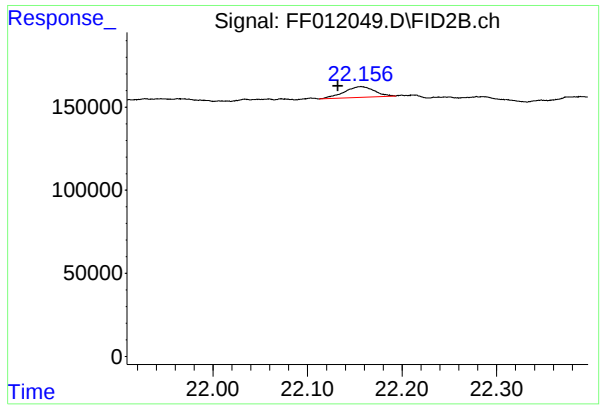

#18 N-TETRACONTANE

R.T.: 22.156 min
Delta R.T.: 0.024 min
Response: 144037
Conc: 1.39 ug/ml

Instrument :

FID_F

ClientSampleId :