

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
 Data File : FF012057.D
 Signal(s) : FID2B.ch
 Acq On : 13 Feb 2023 15:53
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 01:33:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.769	913055	7.622 ug/ml
12) N-OCTACOSANE	17.231	948151	7.291 ug/ml
13) N-TRIACONTANE	18.118	59416	0.460 ug/ml
14) N-DOTRIACONTANE	18.953	94519	0.726 ug/ml
15) N-TETRATRIACONTANE	19.737	34	0.000 ug/ml
16) N-HEXATRIACONTANE	20.477	210489	2.049 ug/ml
17) N-OCTATRIACONTANE	21.222	129832	1.318 ug/ml
18) N-TETRACONTANE	22.149	150629	1.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021323\
Data File : FF012057.D
Signal(s) : FID2B.ch
Acq On : 13 Feb 2023 15:53
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 01:33:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

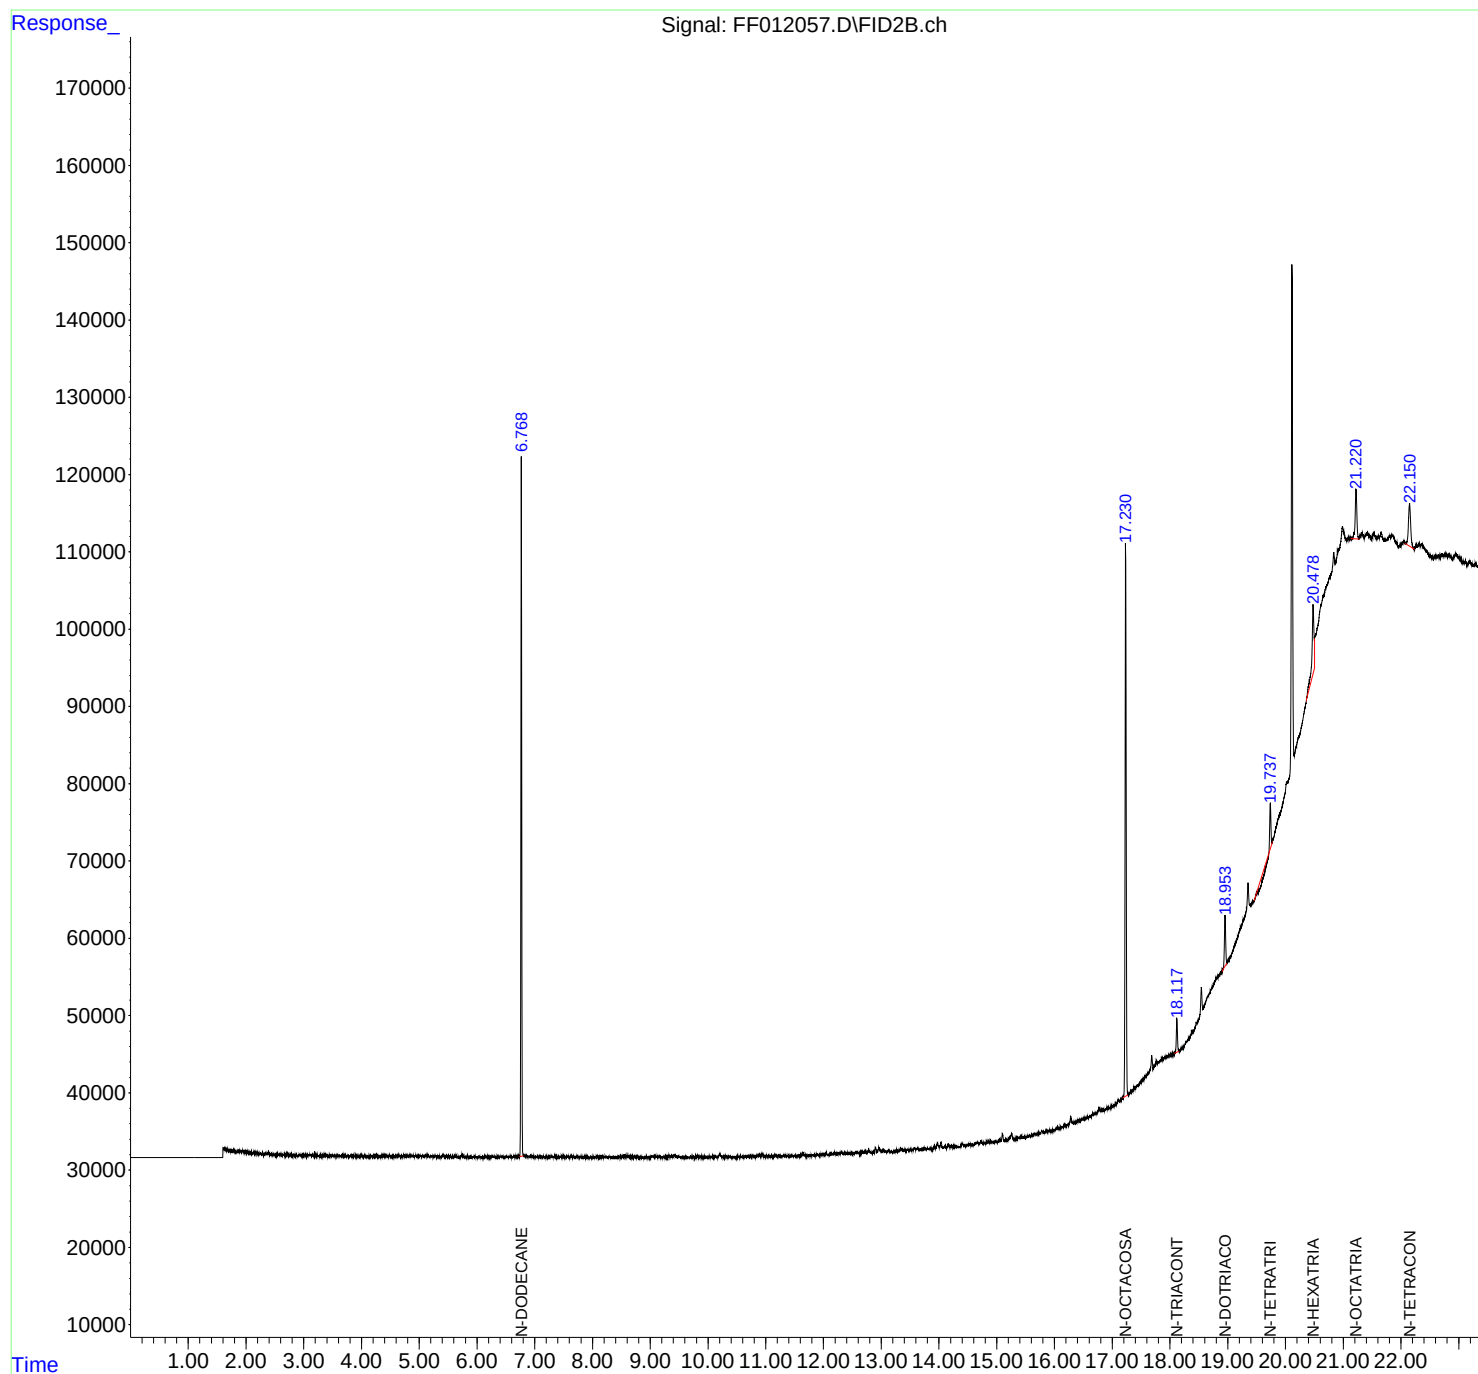


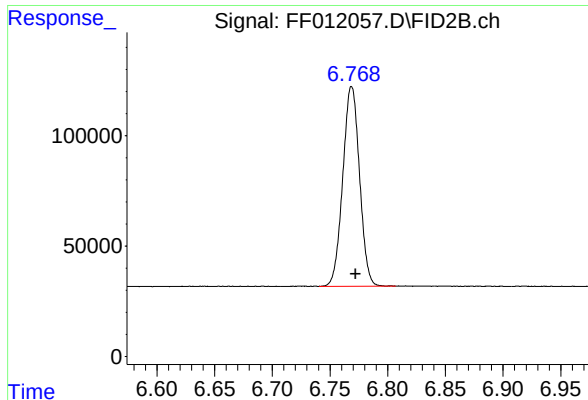

#3 N-DODECANE


R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 913055
Conc: 7.62 ug/ml

Instrument :
FID_F
ClientSampleId :

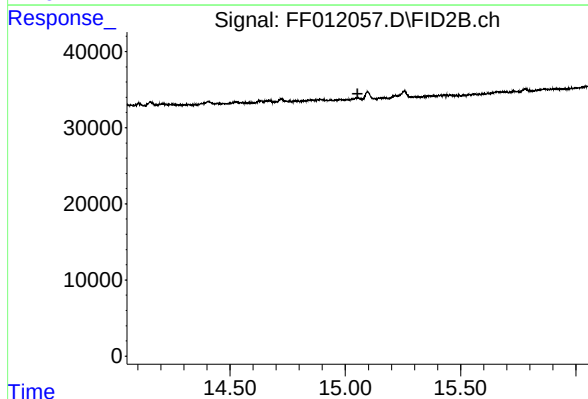


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

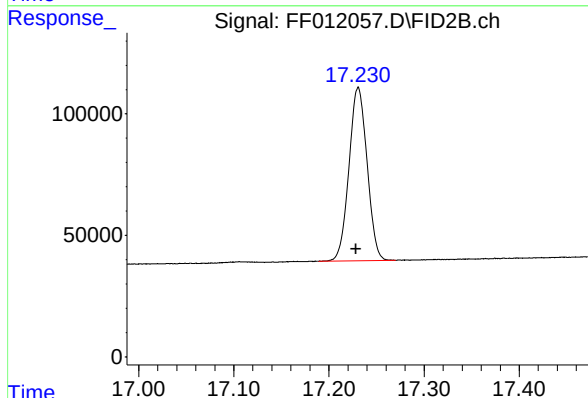


#12 N-OCTACOSANE

R.T.: 17.231 min
Delta R.T.: 0.002 min
Response: 948151
Conc: 7.29 ug/ml

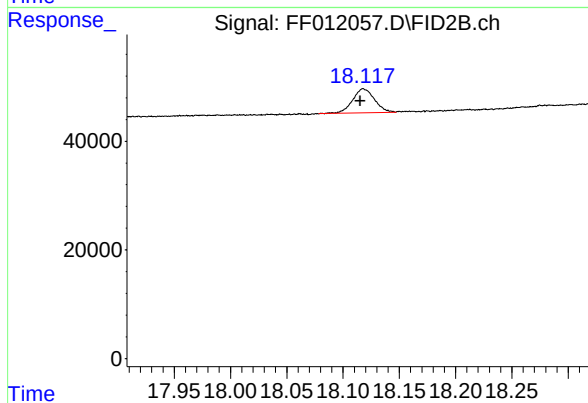

#13 N-TRIACONTANE


R.T.: 18.118 min
Delta R.T.: 0.003 min
Response: 59416
Conc: 0.46 ug/ml

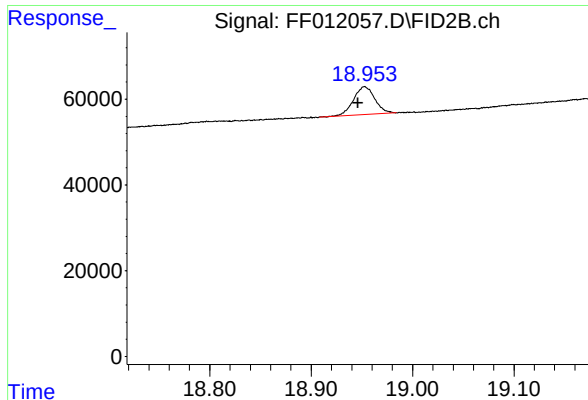

#14 N-DOTRIACONTANE


R.T.: 18.953 min
Delta R.T.: 0.006 min
Response: 94519
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :

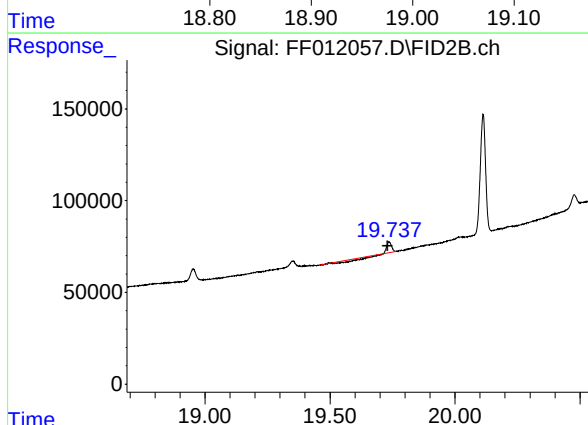


#15 N-TETRATRIACONTANE

R.T.: 19.737 min
Delta R.T.: 0.007 min
Response: 34
Conc: 0.00 ug/ml

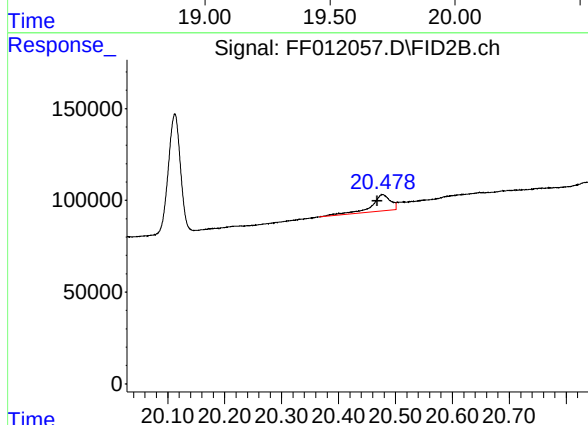


#16 N-HEXATRIACONTANE

R.T.: 20.477 min
Delta R.T.: 0.009 min
Response: 210489
Conc: 2.05 ug/ml

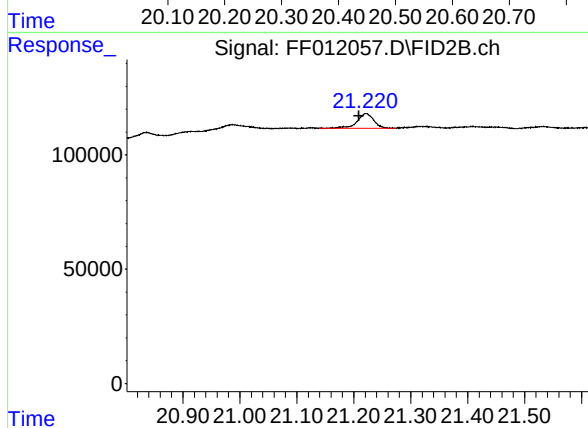

#17 N-OCTATRIACONTANE

R.T.: 21.222 min
Delta R.T.: 0.013 min
Response: 129832
Conc: 1.32 ug/ml

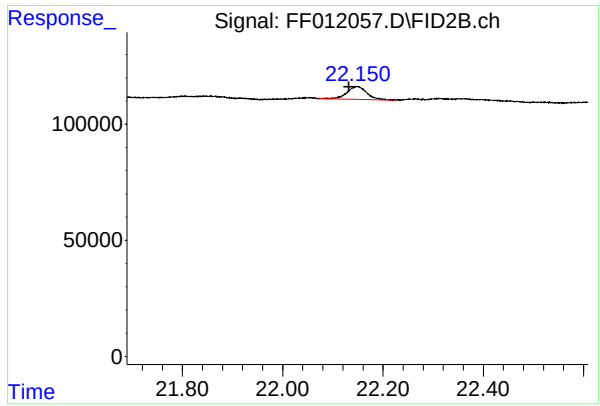

#18 N-TETRACONTANE

R.T.: 22.149 min
Delta R.T.: 0.017 min
Response: 150629
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :