

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006400.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 10:52
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 23:43:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.385	2879559	21.069 ug/ml
12)	N-OCTACOSANE	16.770	2819466	20.430 ug/ml
16)	N-HEXATRIACONTANE	20.033	303677	3.138 ug/ml
18)	N-TETRACONTANE	21.609	470906	6.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006400.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 10:52
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 23:43:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

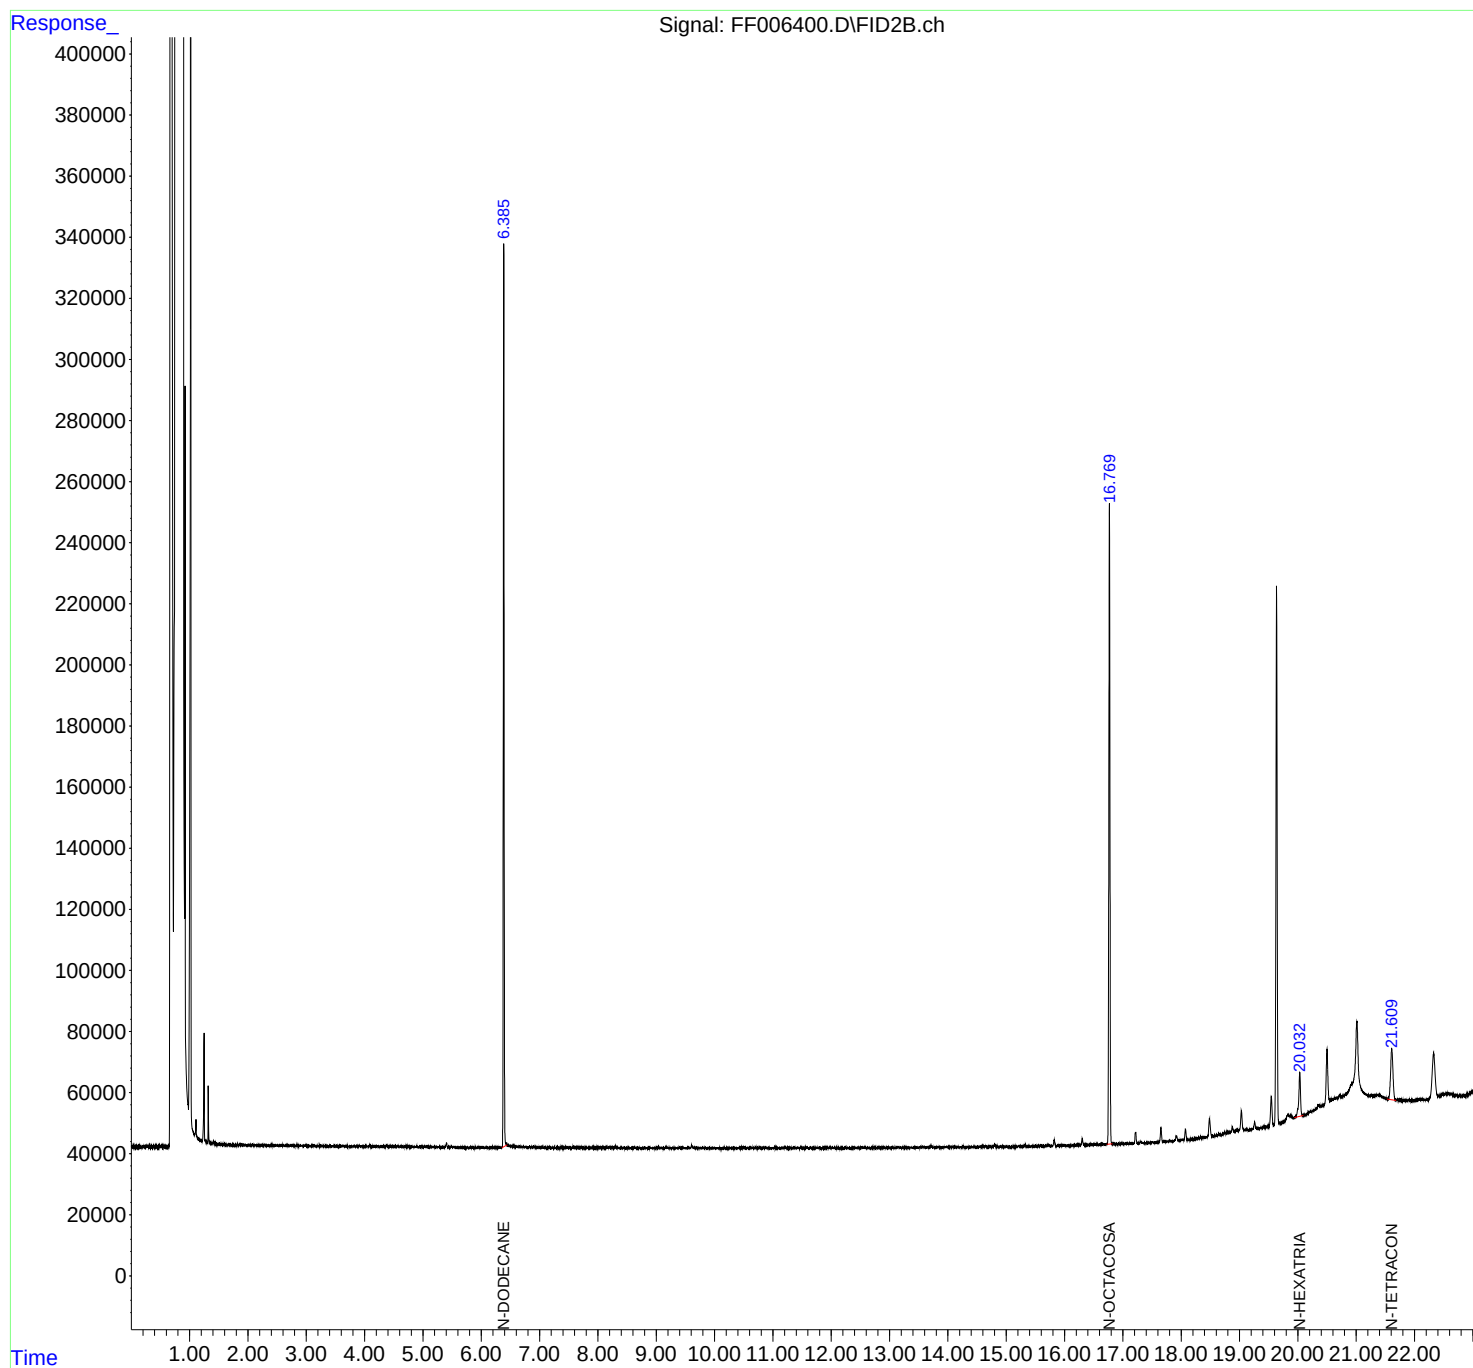


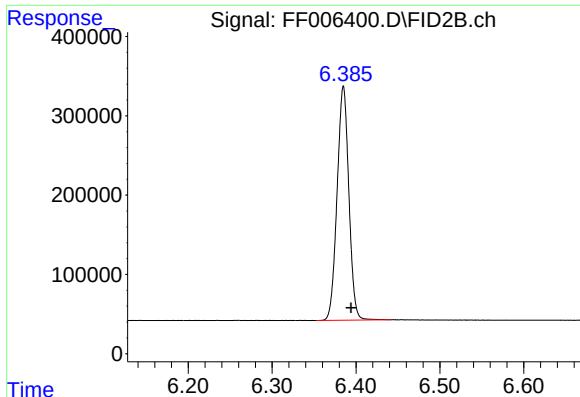

#3 N-DODECANE


R.T.: 6.385 min
Delta R.T.: -0.009 min
Response: 2879559
Conc: 21.07 ug/ml

Instrument :
FID_F
ClientSampleId :

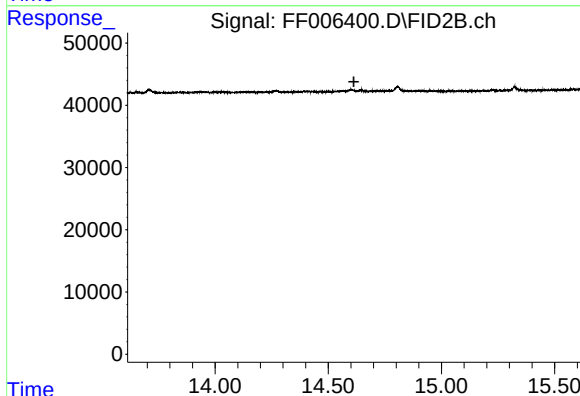


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

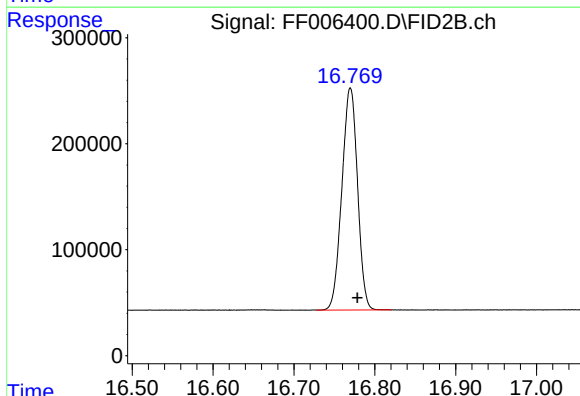


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 2819466
Conc: 20.43 ug/ml

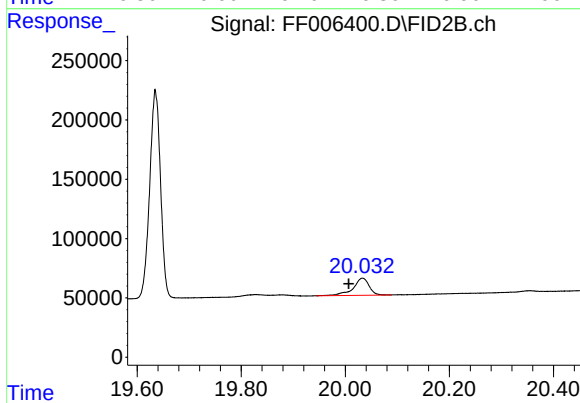

#16 N-HEXATRIACONTANE

R.T.: 20.033 min
Delta R.T.: 0.027 min
Response: 303677
Conc: 3.14 ug/ml

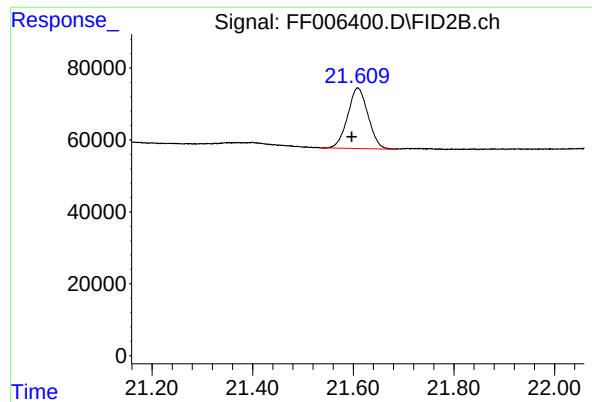

#18 N-TETRACONTANE

R.T.: 21.609 min
Delta R.T.: 0.012 min
Response: 470906
Conc: 6.67 ug/ml

Instrument :
FID_F
ClientSampleId :