

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
 Data File : FF006404.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2020 14:55
 Operator : DD\AJ
 Sample : L1512-02 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 23:43:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	455777	3.741 ug/ml
Target Compounds			
5) N-HEXADECANE	9.789	113194	0.807 ug/ml
7) N-EICOSANE	12.529	140713	0.998 ug/ml
8) N-DOCOSANE	13.744	383939	2.732 ug/ml
10) N-TETRACOSANE	14.796	1298351	9.292 ug/ml
12) N-OCTACOSANE	16.793	348507	2.525 ug/ml
13) N-TRIACONTANE	17.660	293130	2.120 ug/ml
14) N-DOTRIACONTANE	18.483	138476	1.053 ug/ml
15) N-TETRATRIACONTANE	19.305	36429	0.324 ug/ml
16) N-HEXATRIACONTANE	20.019	72937	0.754 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006404.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 14:55
Operator : DD\AJ
Sample : L1512-02 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 14 23:43:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

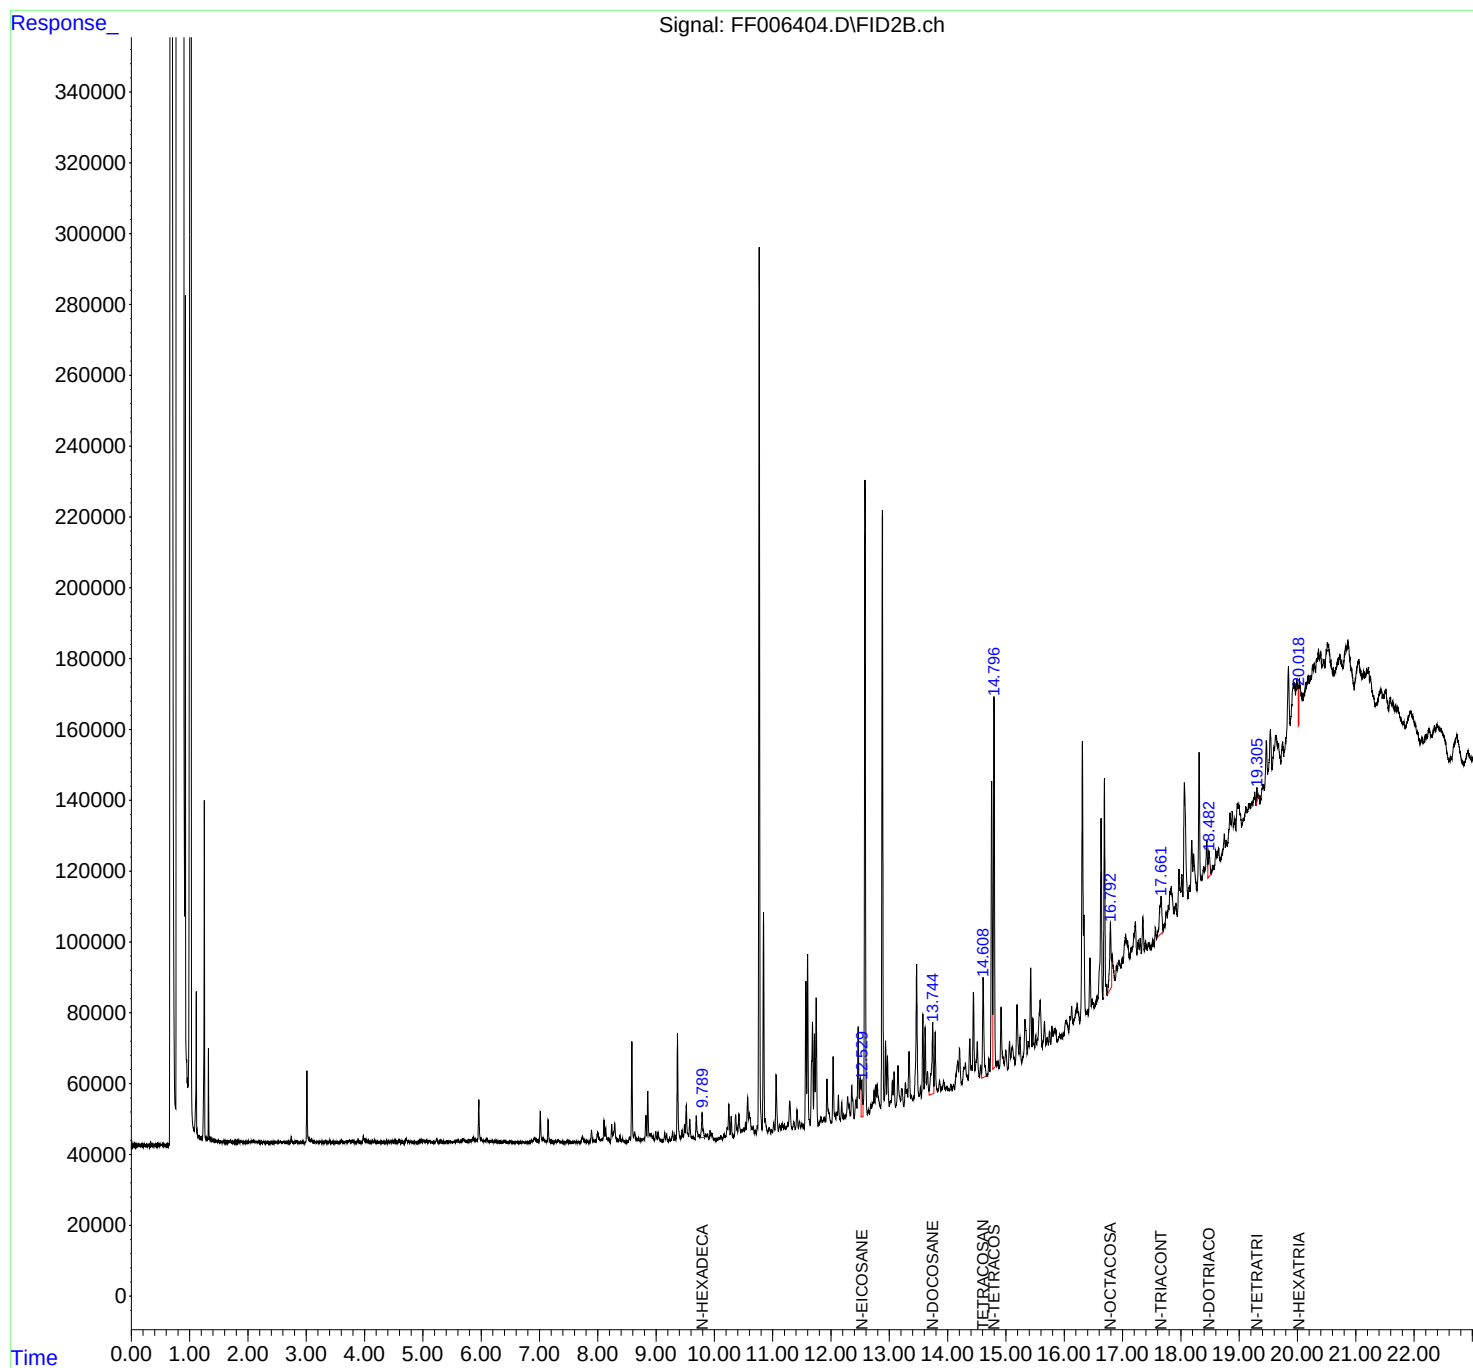


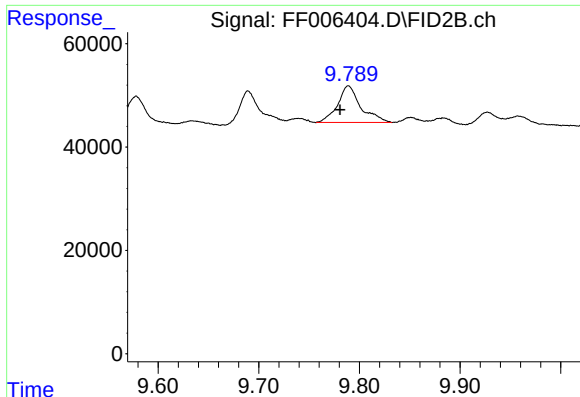

#5 N-HEXADECANE


R.T.: 9.789 min
Delta R.T.: 0.008 min
Response: 113194
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :

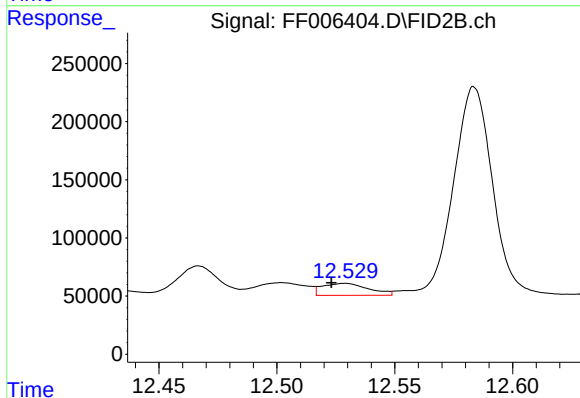


#7 N-EICOSANE

R.T.: 12.529 min
Delta R.T.: 0.006 min
Response: 140713
Conc: 1.00 ug/ml

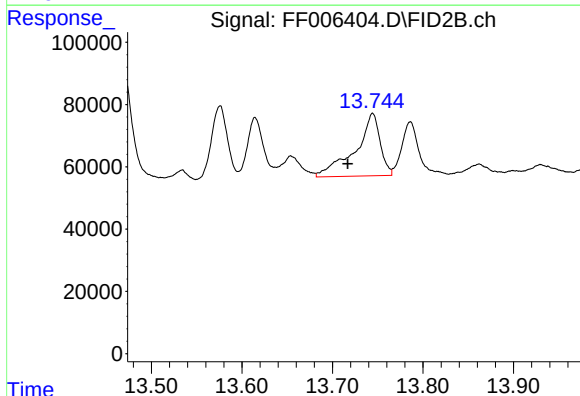


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: 0.028 min
Response: 383939
Conc: 2.73 ug/ml

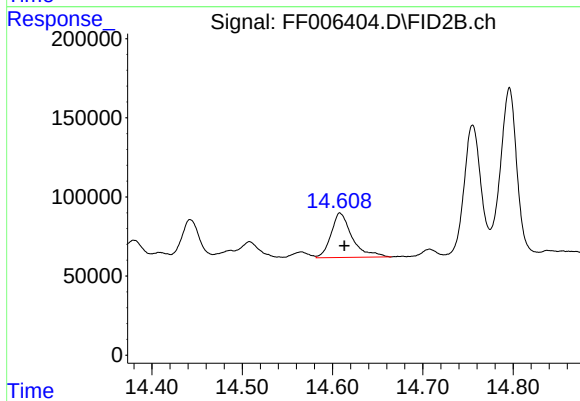

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.608 min
Delta R.T.: -0.005 min
Response: 455777
Conc: 3.74 ug/ml

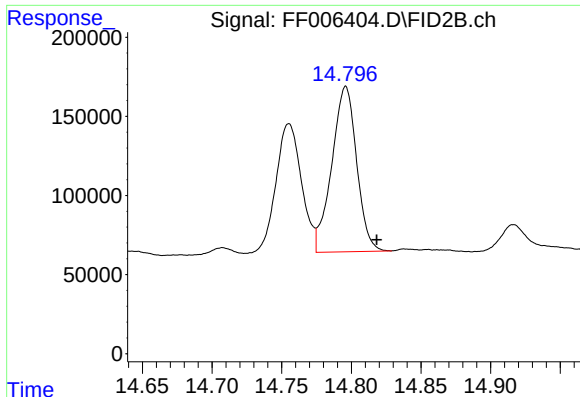

#10 N-TETRACOSANE


R.T.: 14.796 min
Delta R.T.: -0.022 min
Response: 1298351
Conc: 9.29 ug/ml

Instrument :
FID_F
ClientSampleId :

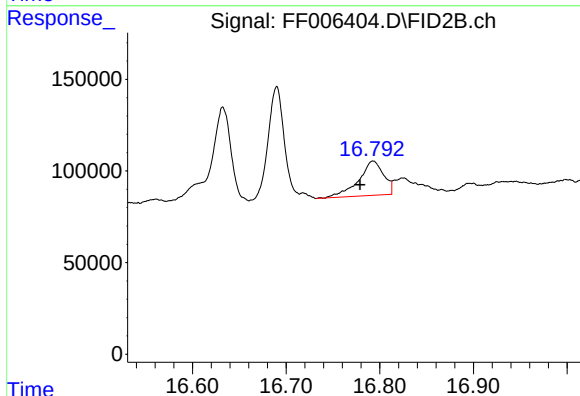


#12 N-OCTACOSANE

R.T.: 16.793 min
Delta R.T.: 0.014 min
Response: 348507
Conc: 2.53 ug/ml

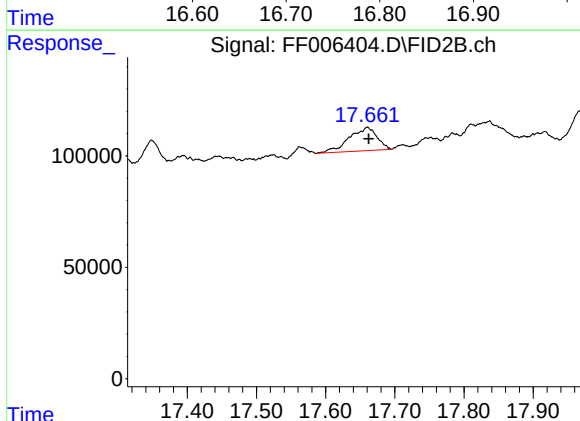


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.002 min
Response: 293130
Conc: 2.12 ug/ml

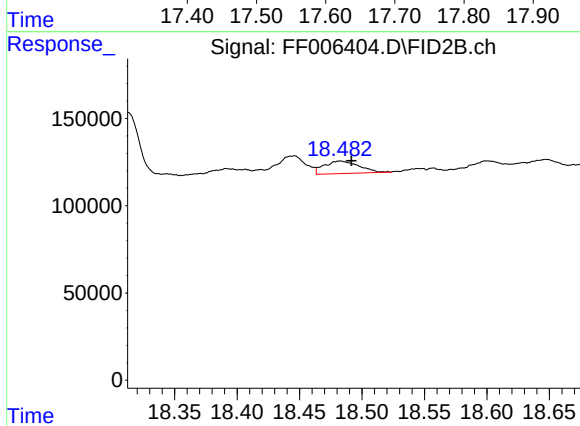

#14 N-DOTRIACONTANE


R.T.: 18.483 min
Delta R.T.: -0.009 min
Response: 138476
Conc: 1.05 ug/ml

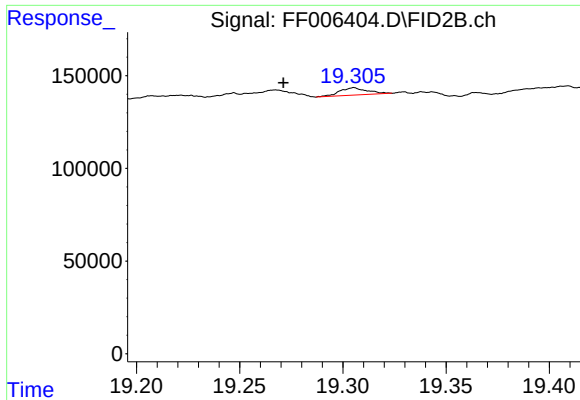

#15 N-TETRATRIACONTANE

R.T.: 19.305 min
Delta R.T.: 0.034 min
Response: 36429
Conc: 0.32 ug/ml

Instrument :
FID_F
ClientSampleId :

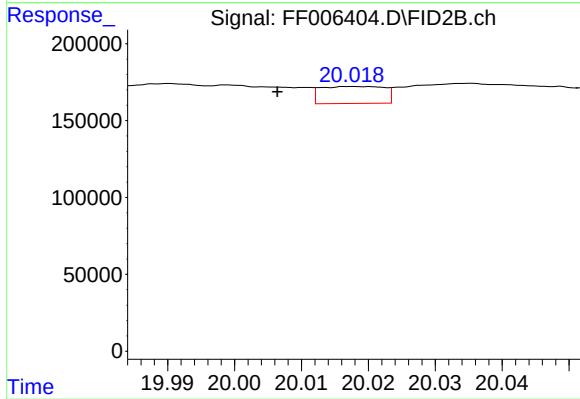

#16 N-HEXATRIACONTANE

R.T.: 20.019 min
Delta R.T.: 0.012 min
Response: 72937
Conc: 0.75 ug/ml