

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
 Data File : FF006405.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2020 15:25
 Operator : DD\AJ
 Sample : L1512-02 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 23:43:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.607	242935	1.994 ug/ml
Target Compounds			
7) N-EICOSANE	12.466f	120042	0.852 ug/ml
8) N-DOCOSANE	13.744	199887	1.422 ug/ml
10) N-TETRACOSANE	14.794	808128	5.783 ug/ml
12) N-OCTACOSANE	16.792	105693	0.766 ug/ml
13) N-TRIACONTANE	17.658	192427	1.391 ug/ml
14) N-DOTRIACONTANE	18.490	115729	0.880 ug/ml
16) N-HEXATRIACONTANE	19.992	152364	1.574 ug/ml
17) N-OCTATRIACONTANE	20.738	278873	3.949 ug/ml
18) N-TETRACONTANE	21.624	351789	4.984 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006405.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 15:25
Operator : DD\AJ
Sample : L1512-02 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 14 23:43:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

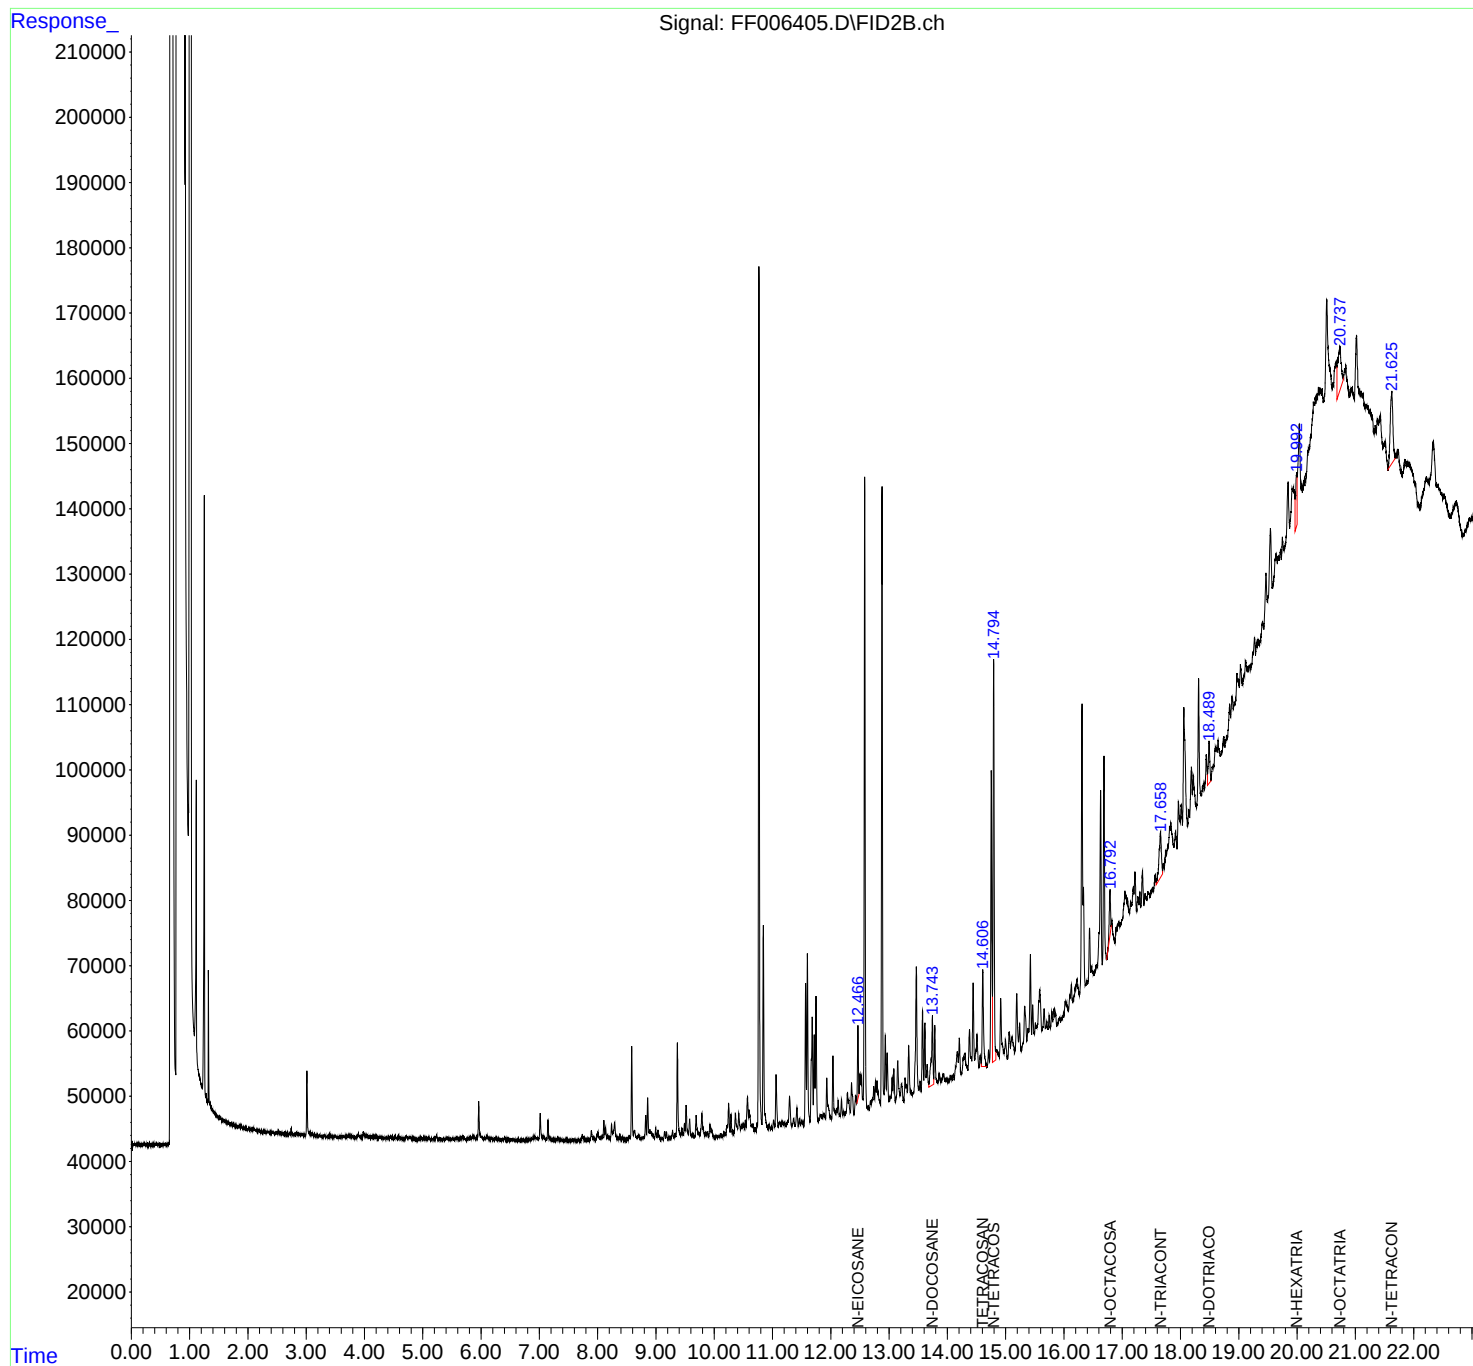


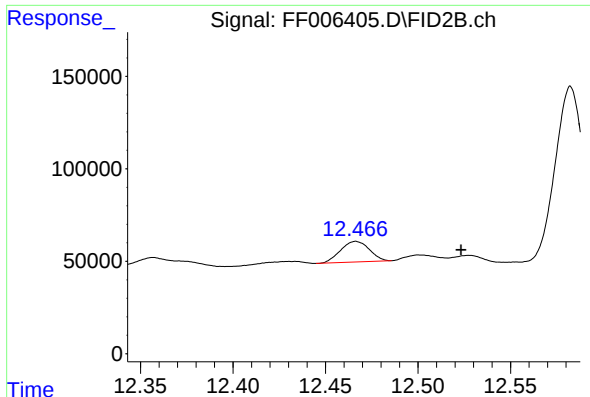

#7 N-EICOSANE


R.T.: 12.466 min
Delta R.T.: -0.057 min
Response: 120042
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

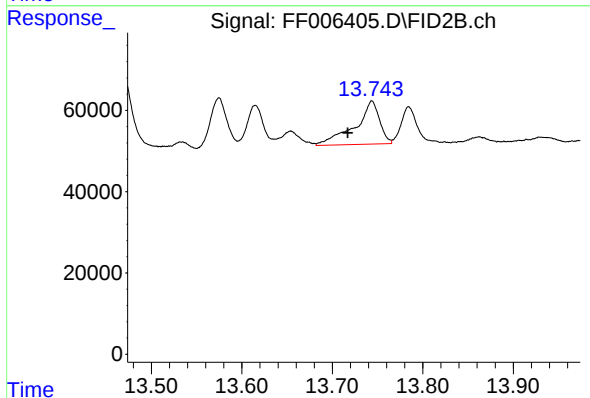


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: 0.027 min
Response: 199887
Conc: 1.42 ug/ml

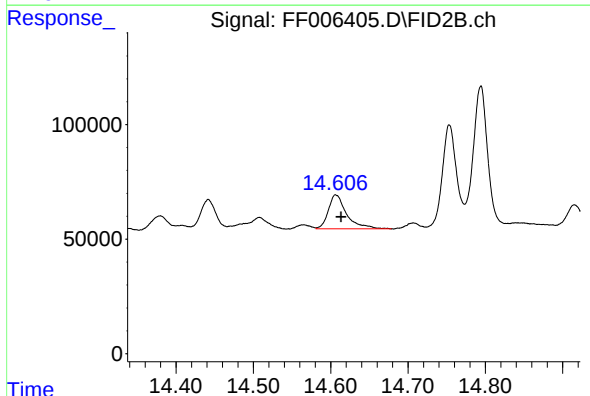


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.607 min
Delta R.T.: -0.007 min
Response: 242935
Conc: 1.99 ug/ml

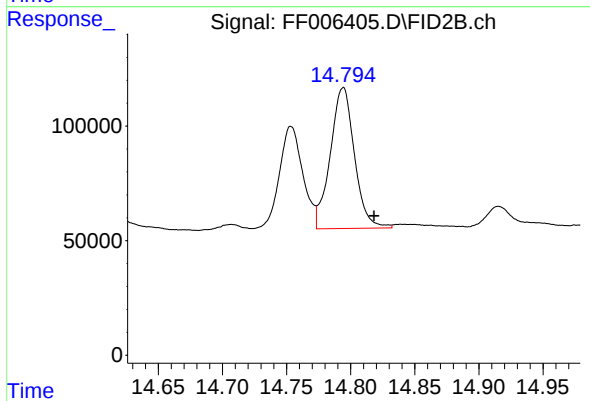

#10 N-TETRACOSANE


R.T.: 14.794 min
Delta R.T.: -0.024 min
Response: 808128
Conc: 5.78 ug/ml

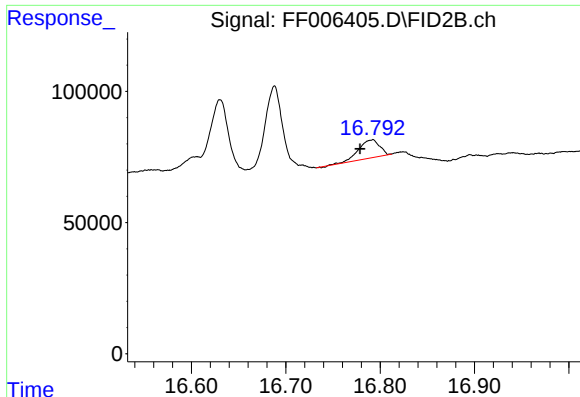

#12 N-OCTACOSANE


R.T.: 16.792 min
Delta R.T.: 0.013 min
Response: 105693
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :

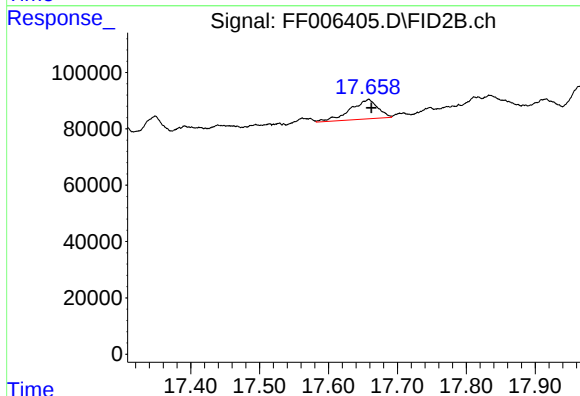


#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: -0.004 min
Response: 192427
Conc: 1.39 ug/ml

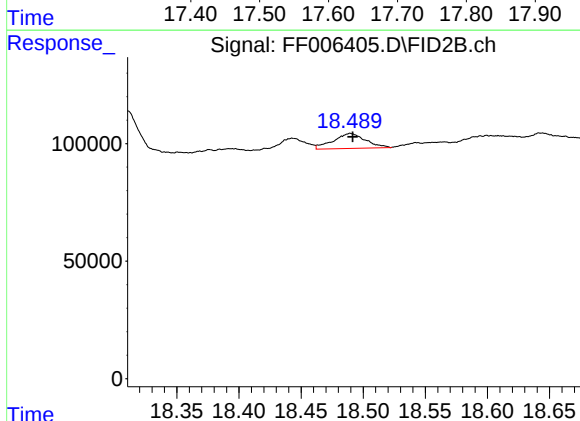


#14 N-DOTRIACONTANE

R.T.: 18.490 min
Delta R.T.: -0.002 min
Response: 115729
Conc: 0.88 ug/ml

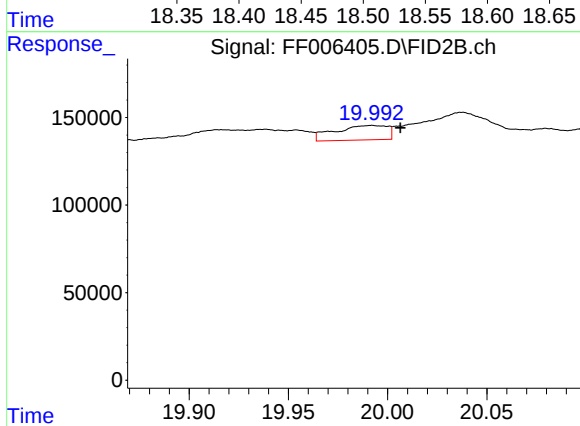

#16 N-HEXATRIACONTANE


R.T.: 19.992 min
Delta R.T.: -0.014 min
Response: 152364
Conc: 1.57 ug/ml

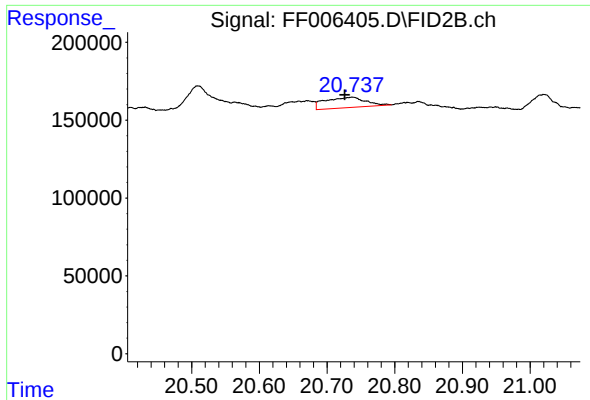

#17 N-OCTATRIACONTANE

R.T.: 20.738 min
Delta R.T.: 0.011 min
Response: 278873
Conc: 3.95 ug/ml

Instrument :
FID_F
ClientSampleId :

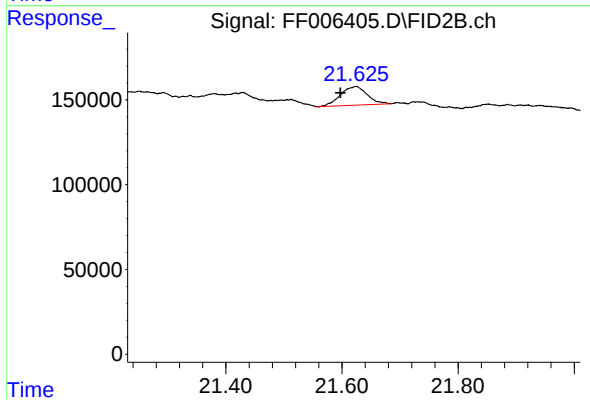

#18 N-TETRACONTANE

R.T.: 21.624 min
Delta R.T.: 0.027 min
Response: 351789
Conc: 4.98 ug/ml