

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
 Data File : FF006409.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2020 17:25
 Operator : DD\AJ
 Sample : L1525-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 23:44:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.610	1823278	14.966 ug/ml
Target Compounds			
4) N-TETRADECANE	8.148	560854	4.077 ug/ml
10) N-TETRACOSANE	14.795	249377	1.785 ug/ml
12) N-OCTACOSANE	16.776	168018	1.217 ug/ml
13) N-TRIACONTANE	17.659	222157	1.606 ug/ml
14) N-DOTRIACONTANE	18.484	624330	4.745 ug/ml
15) N-TETRATRIACONTANE	19.268	156614	1.395 ug/ml
16) N-HEXATRIACONTANE	20.009	90327	0.933 ug/ml
17) N-OCTATRIACONTANE	20.724	55772	0.790 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006409.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 17:25
Operator : DD\AJ
Sample : L1525-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 23:44:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

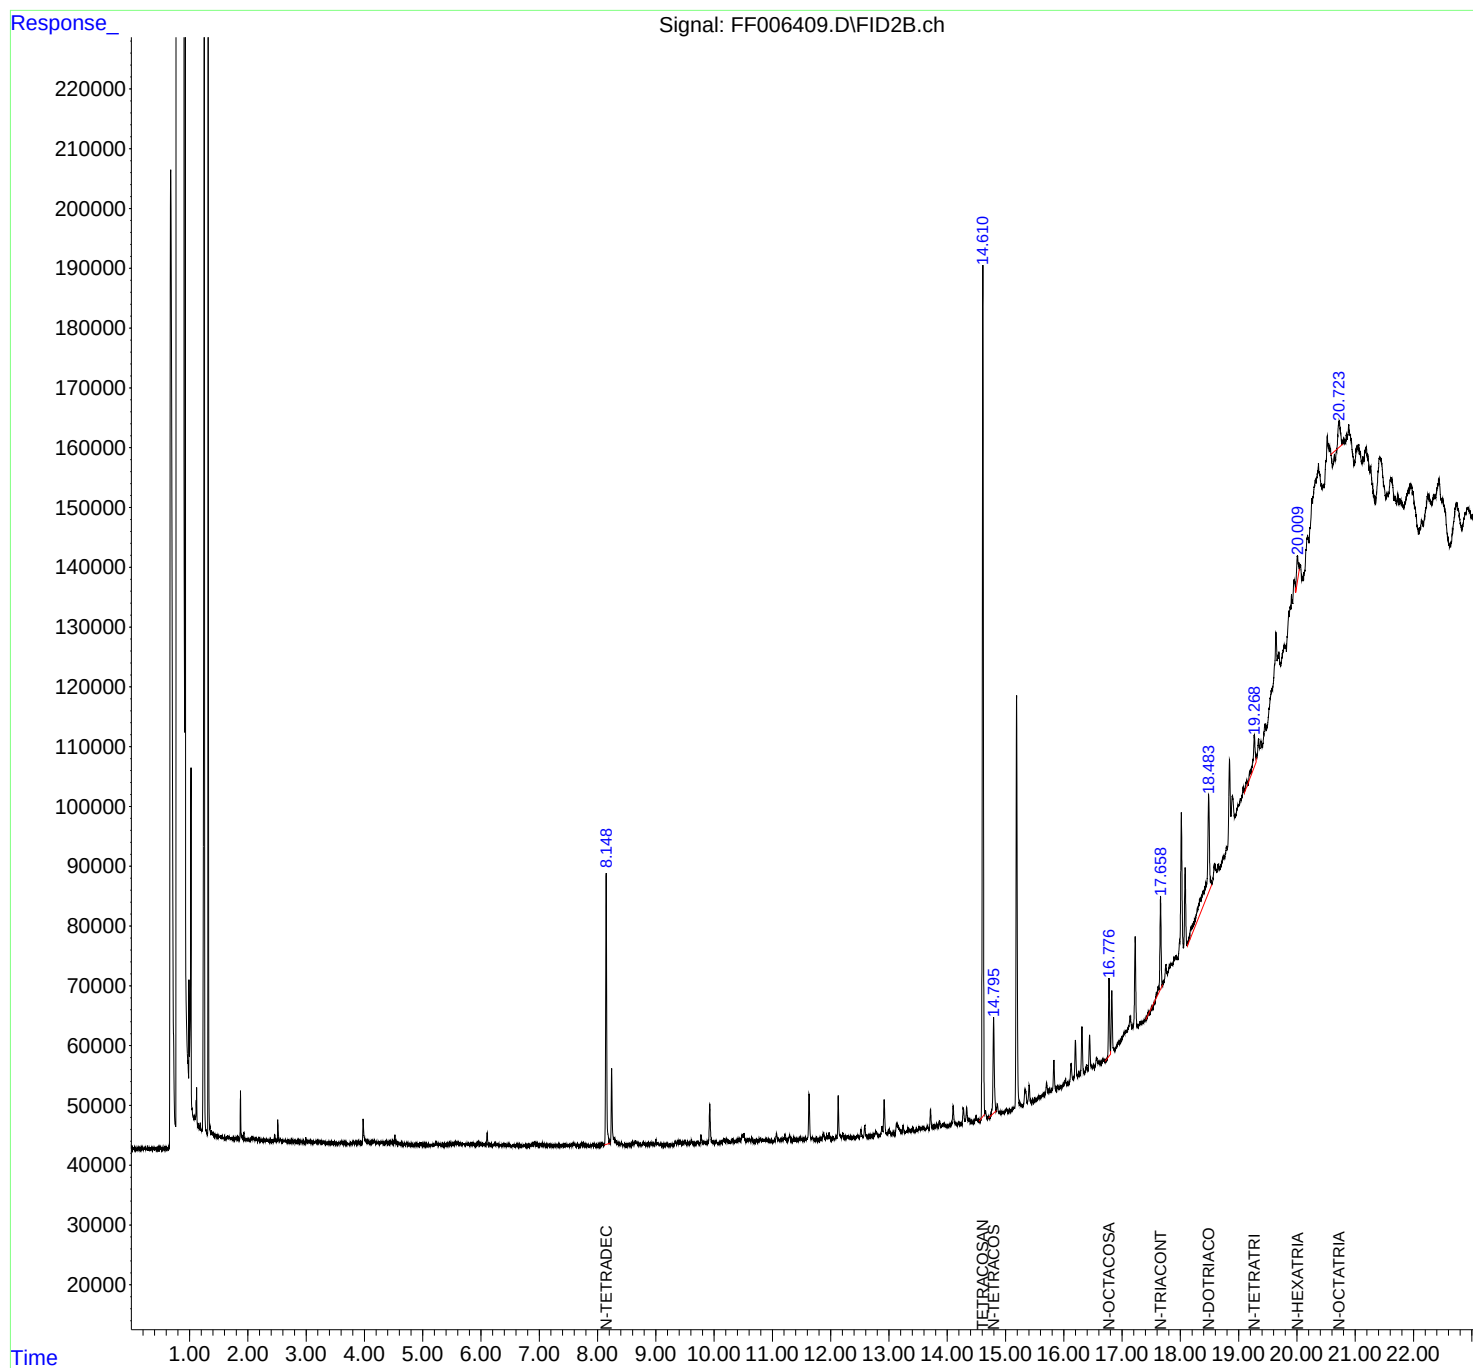


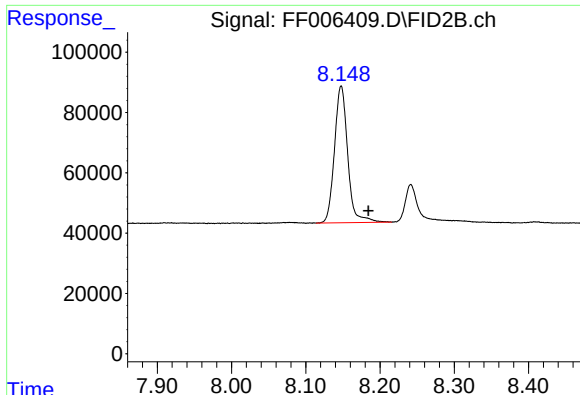

#4 N-TETRADECANE


R.T.: 8.148 min
Delta R.T.: -0.037 min
Response: 560854
Conc: 4.08 ug/ml

Instrument :
FID_F
ClientSampleId :

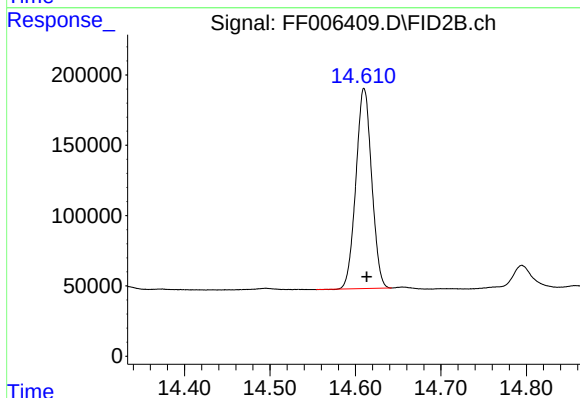


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.610 min
Delta R.T.: -0.003 min
Response: 1823278
Conc: 14.97 ug/ml

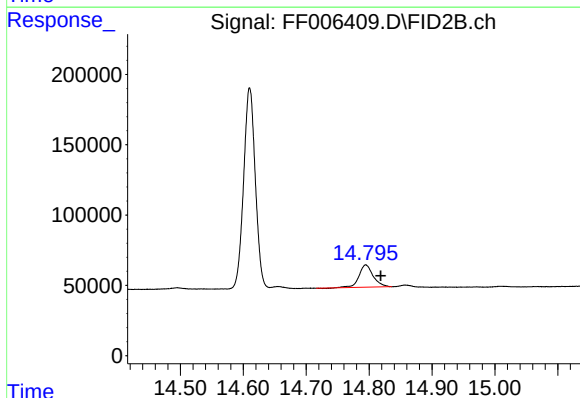


#10 N-TETRACOSANE

R.T.: 14.795 min
Delta R.T.: -0.023 min
Response: 249377
Conc: 1.78 ug/ml

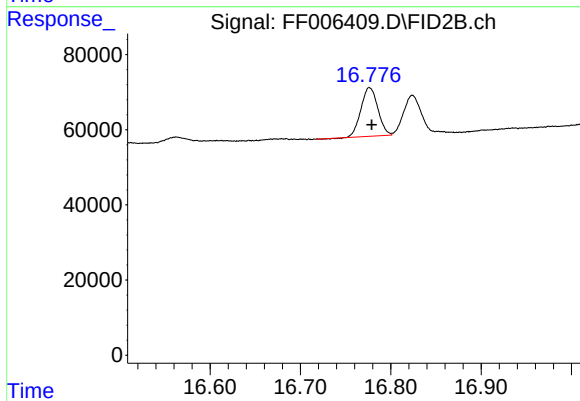

#12 N-OCTACOSANE


R.T.: 16.776 min
Delta R.T.: -0.002 min
Response: 168018
Conc: 1.22 ug/ml

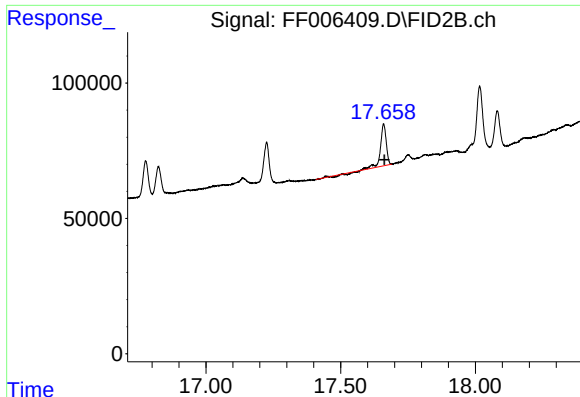

#13 N-TRIACONTANE


R.T.: 17.659 min
Delta R.T.: -0.003 min
Response: 222157
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :

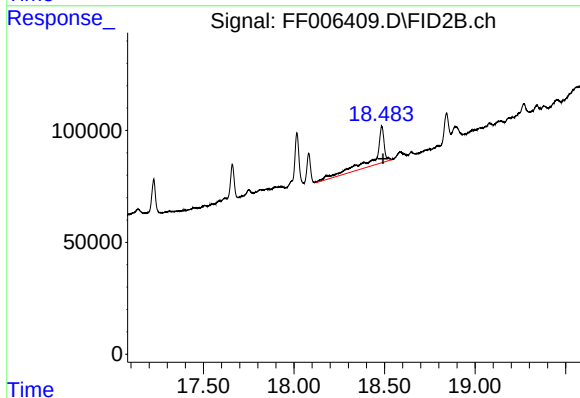


#14 N-DOTRIACONTANE

R.T.: 18.484 min
Delta R.T.: -0.007 min
Response: 624330
Conc: 4.75 ug/ml

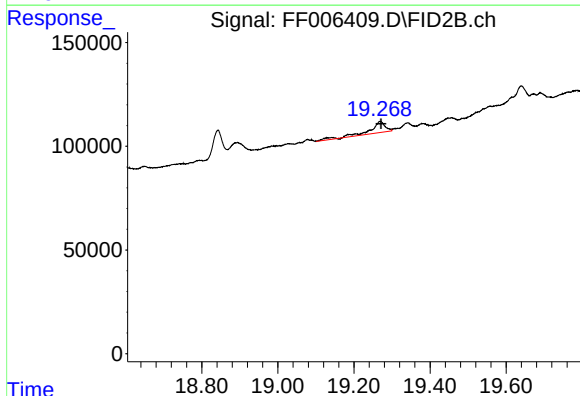


#15 N-TETRATRIACONTANE

R.T.: 19.268 min
Delta R.T.: -0.003 min
Response: 156614
Conc: 1.39 ug/ml

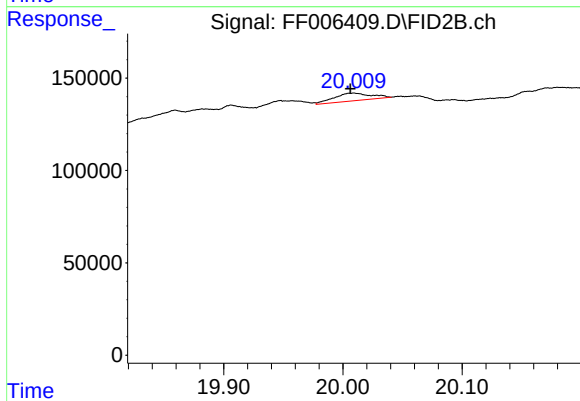

#16 N-HEXATRIACONTANE

R.T.: 20.009 min
Delta R.T.: 0.002 min
Response: 90327
Conc: 0.93 ug/ml

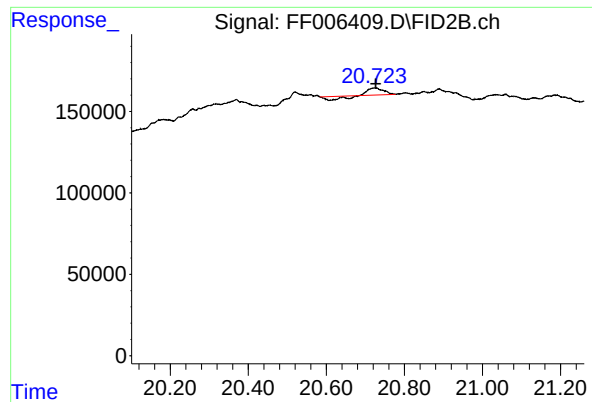

#17 N-OCTATRIACONTANE

R.T.: 20.724 min
Delta R.T.: -0.002 min
Response: 55772
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :