

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
 Data File : FF006410.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2020 17:55
 Operator : DD\AJ
 Sample : PB126817BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 23:44:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.610	2003110	16.442 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.795	214873	1.538 ug/ml
14) N-DOTRIACONTANE	18.486	90011	0.684 ug/ml
15) N-TETRATRIACONTANE	19.265	325899	2.902 ug/ml
16) N-HEXATRIACONTANE	20.033	130314	1.346 ug/ml
17) N-OCTATRIACONTANE	20.730	547325	7.751 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006410.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 17:55
Operator : DD\AJ
Sample : PB126817BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 23:44:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

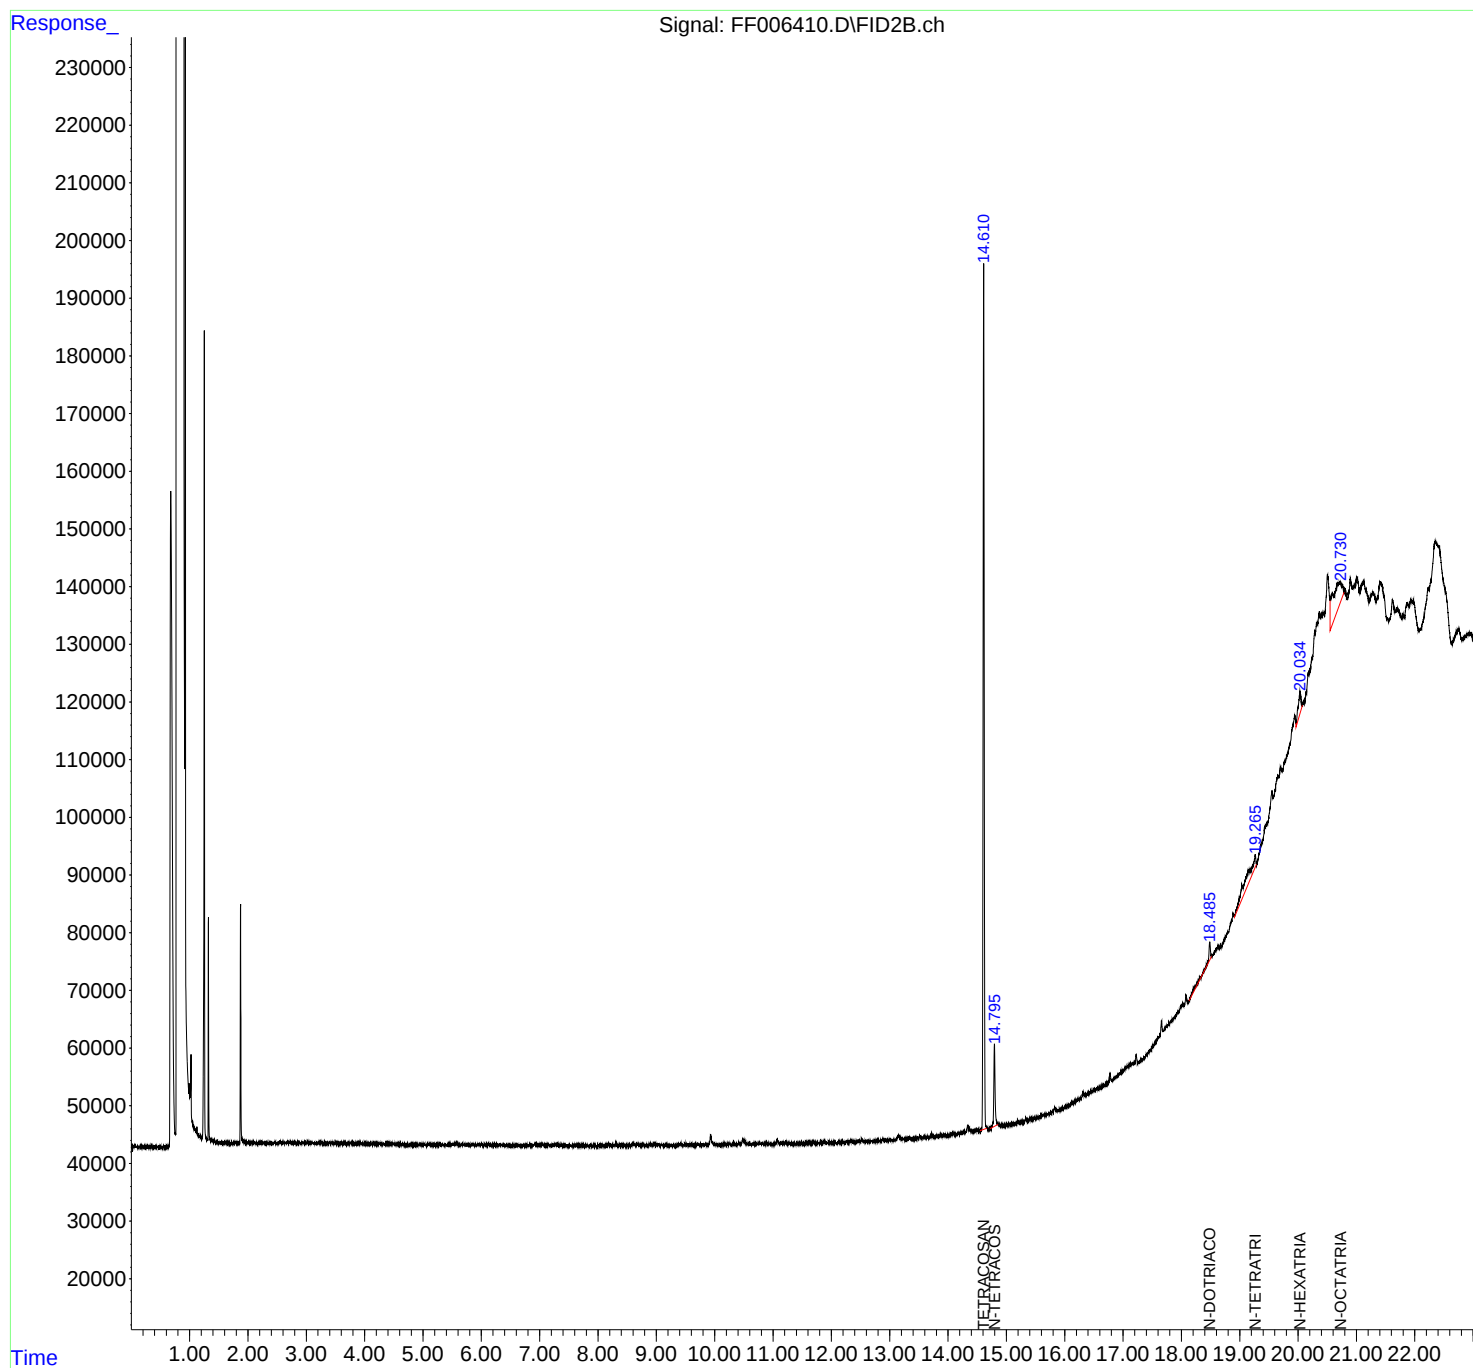


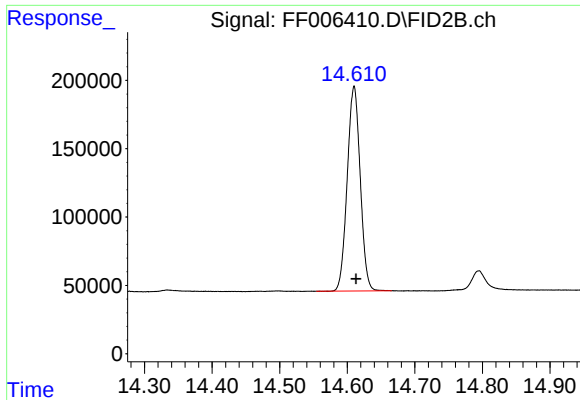

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.610 min
Delta R.T.: -0.003 min
Response: 2003110
Conc: 16.44 ug/ml

Instrument :
FID_F
ClientSampleId :

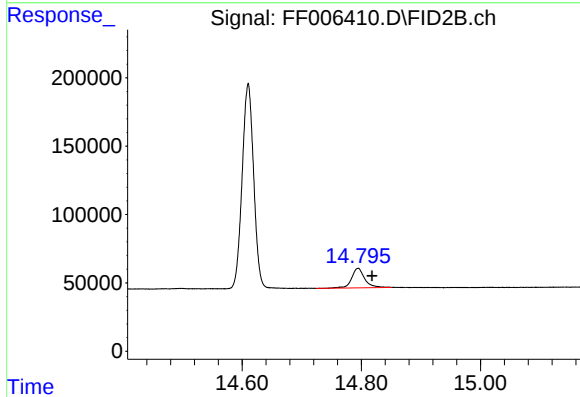


#10 N-TETRACOSANE

R.T.: 14.795 min
Delta R.T.: -0.024 min
Response: 214873
Conc: 1.54 ug/ml

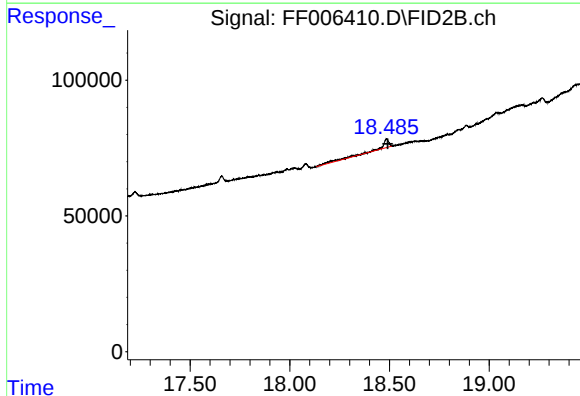


#14 N-DOTRIACONTANE

R.T.: 18.486 min
Delta R.T.: -0.006 min
Response: 90011
Conc: 0.68 ug/ml

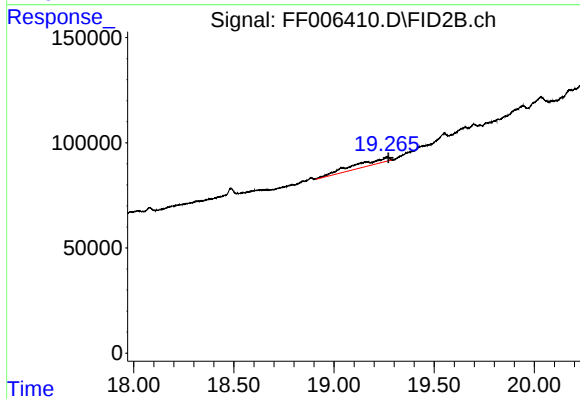

#15 N-TETRATRIACONTANE


R.T.: 19.265 min
Delta R.T.: -0.006 min
Response: 325899
Conc: 2.90 ug/ml

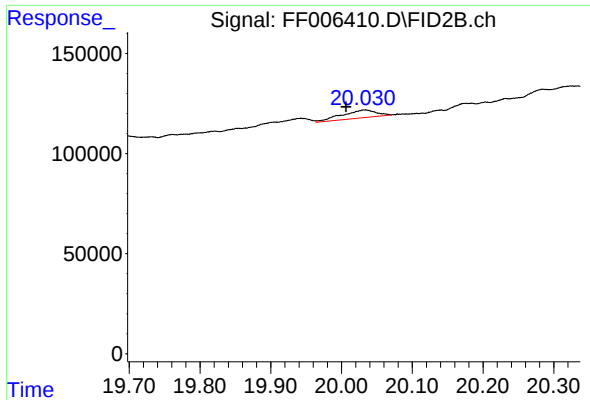

#16 N-HEXATRIACONTANE

R.T.: 20.033 min
Delta R.T.: 0.027 min
Response: 130314
Conc: 1.35 ug/ml

Instrument :
FID_F
ClientSampleId :

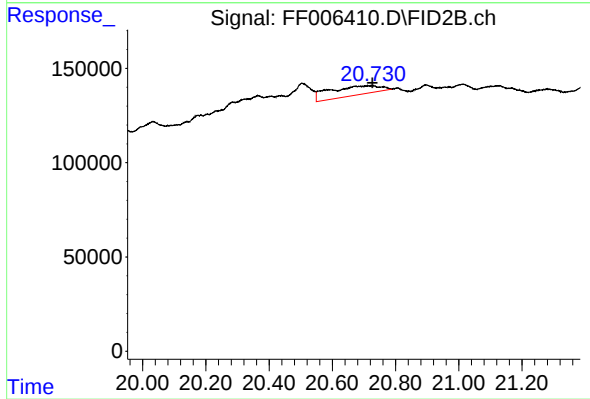

#17 N-OCTATRIACONTANE

R.T.: 20.730 min
Delta R.T.: 0.004 min
Response: 547325
Conc: 7.75 ug/ml