

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006408.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 16:55
Operator : DD\AJ
Sample : L1525-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-1A-(7.5-9.5)

Integration File: autoint1.e
Quant Time: Feb 14 23:44:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1789911	14.692 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021420\
Data File : FF006408.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2020 16:55
Operator : DD\AJ
Sample : L1525-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-1A-(7.5-9.5)

Integration File: autoint1.e
Quant Time: Feb 14 23:44:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

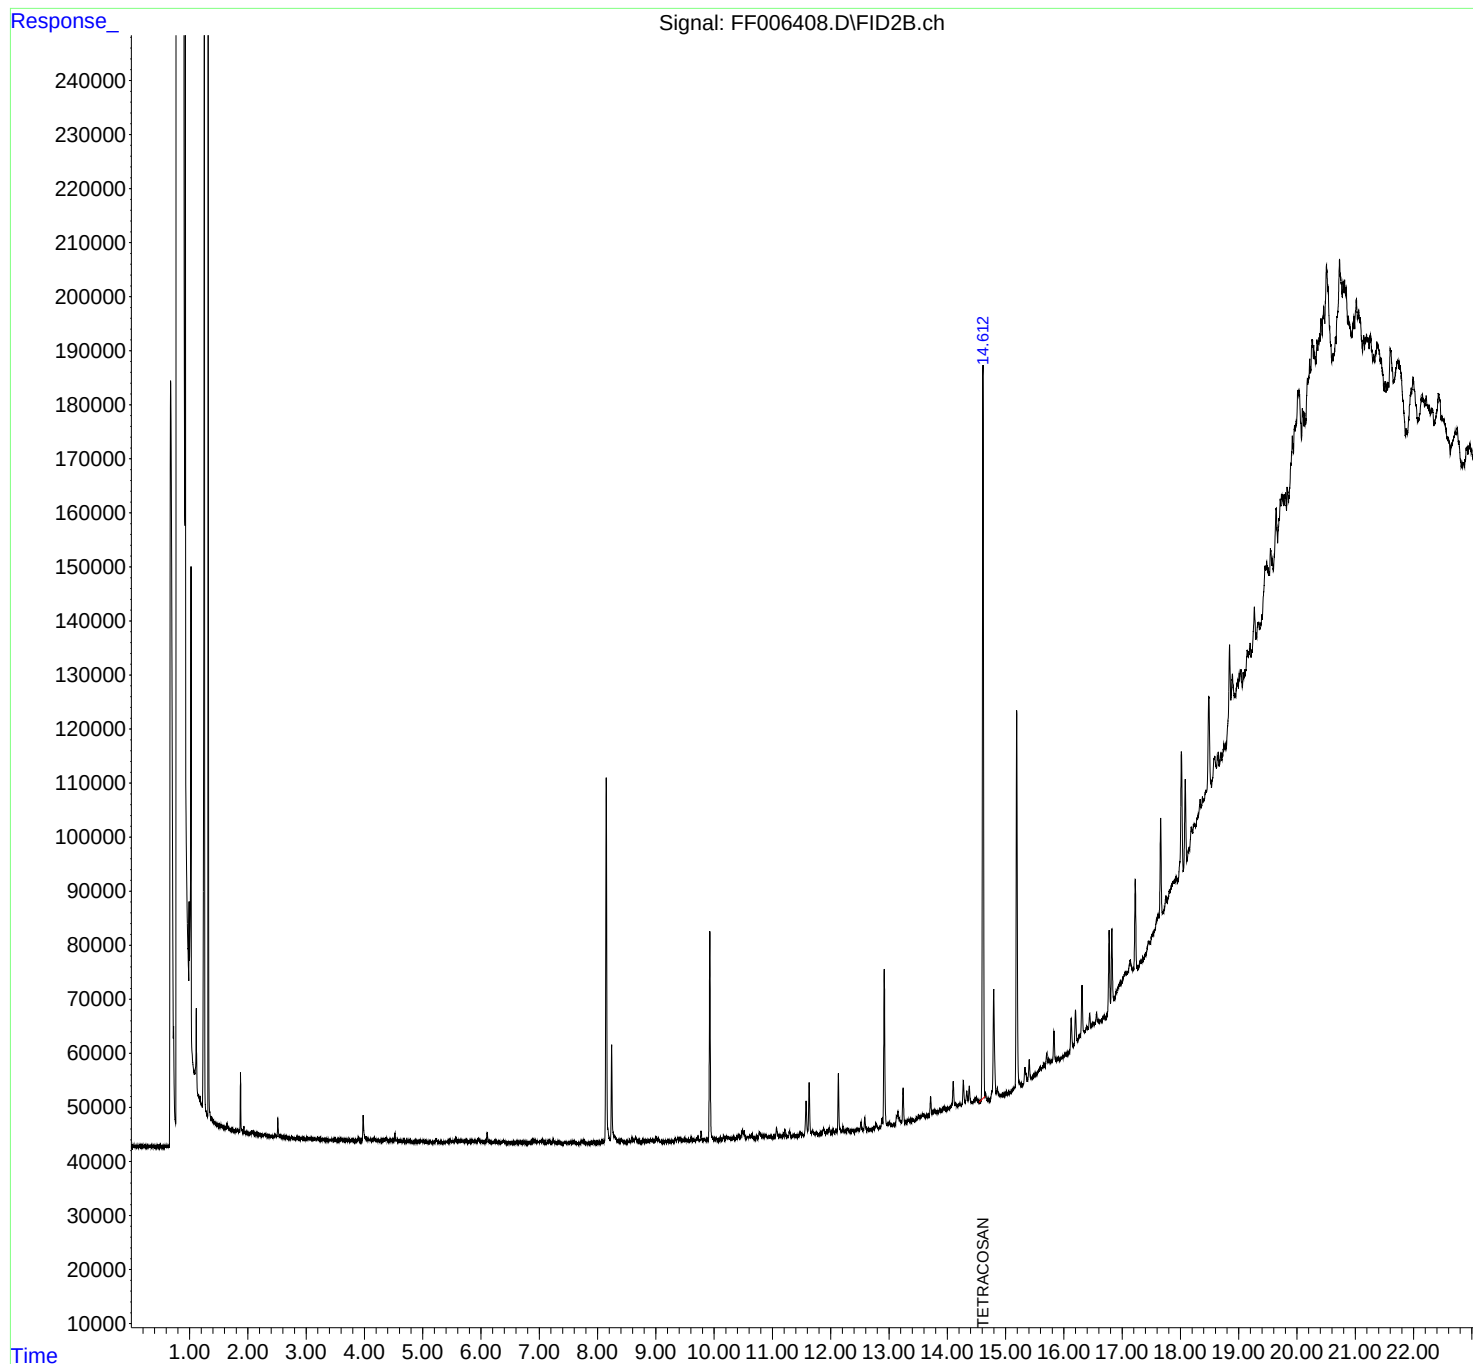

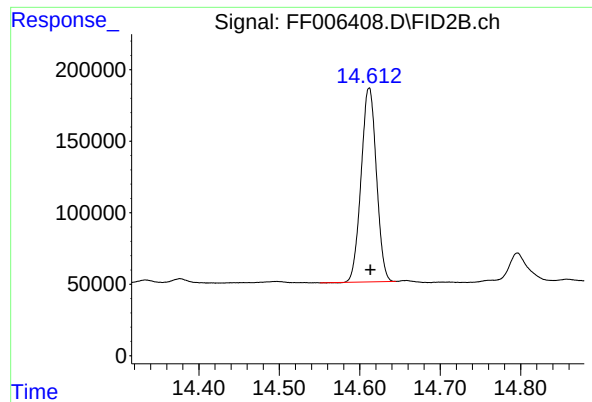

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.002 min
Response: 1789911
Conc: 14.69 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-1A-(7.5-9.5)