

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009933.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 12:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:42:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.209	3651886	26.567 ug/ml
12)	N-OCTACOSANE	16.586	3093469	26.359 ug/ml
13)	N-TRIACONTANE	17.470	63541	0.548 ug/ml
14)	N-DOTRIACONTANE	18.301	97343	0.841 ug/ml
15)	N-TETRATRIACONTANE	19.079	57940	0.518 ug/ml
16)	N-HEXATRIACONTANE	19.860	65082	0.618 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009933.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 12:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:42:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

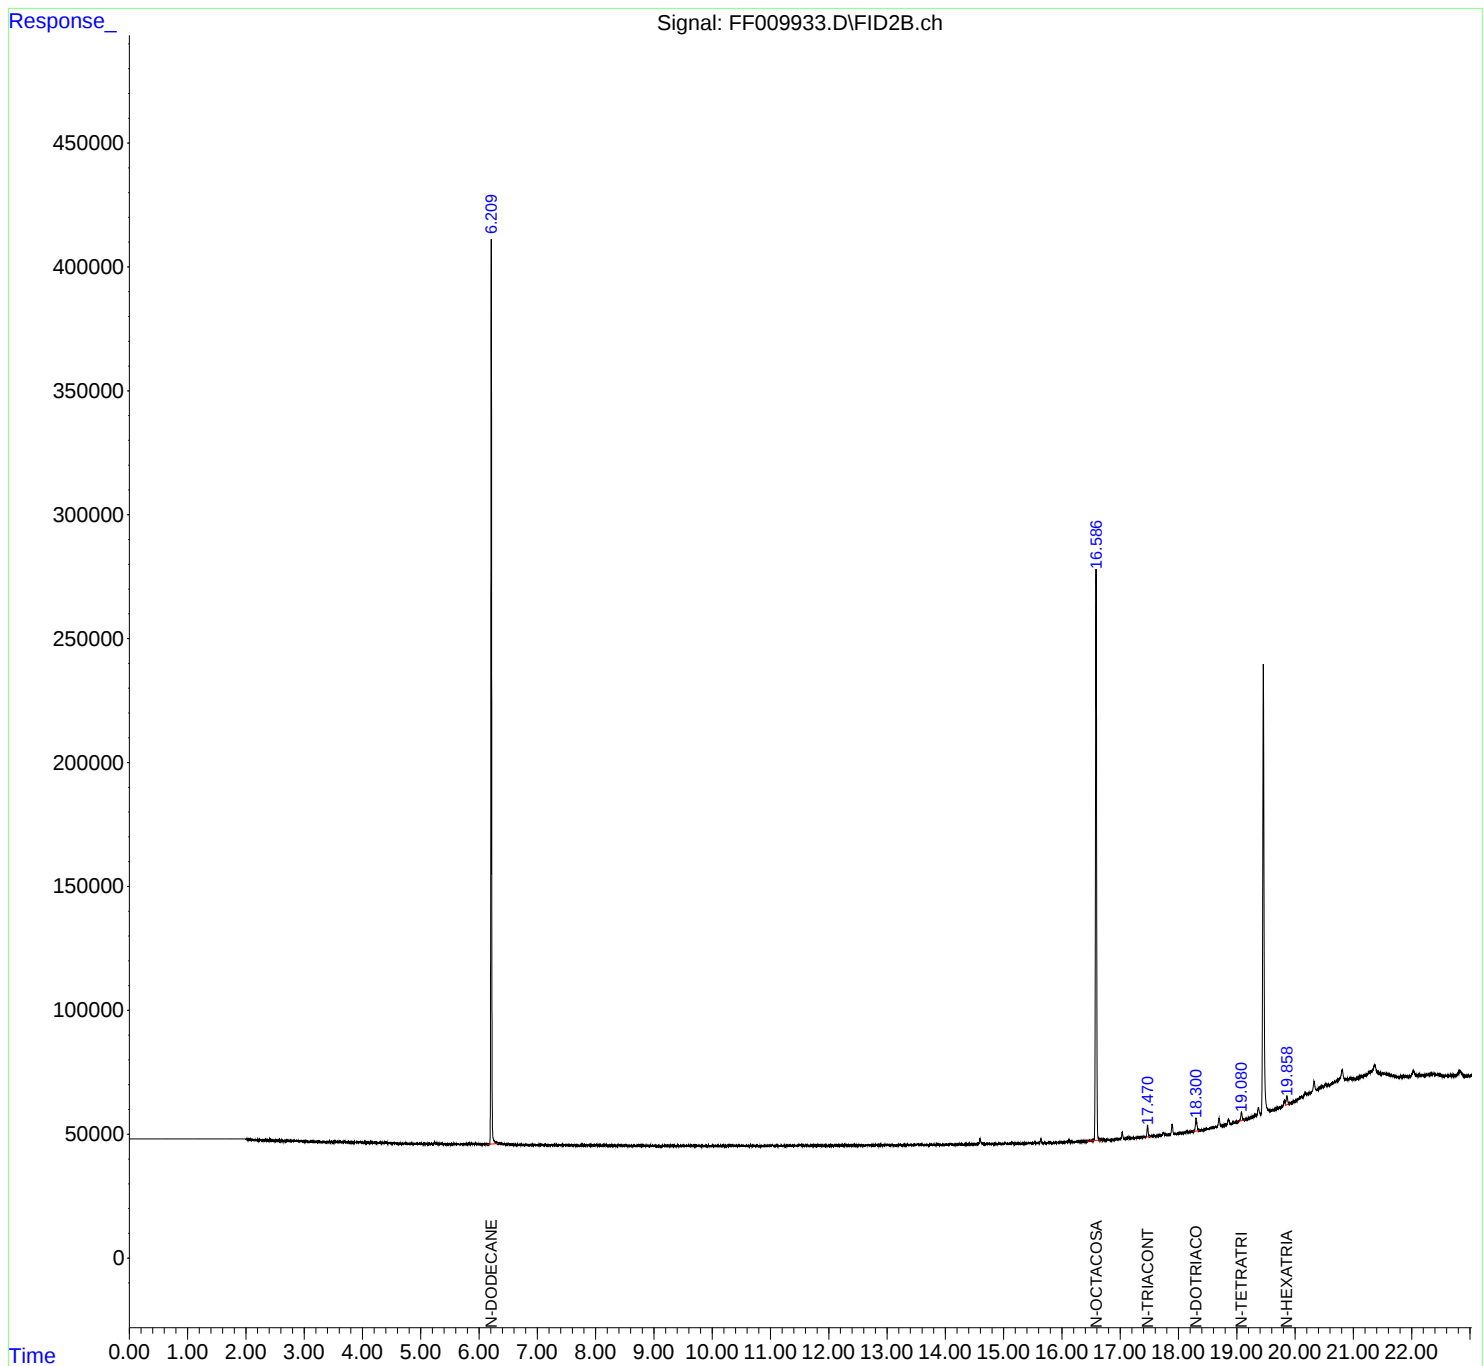


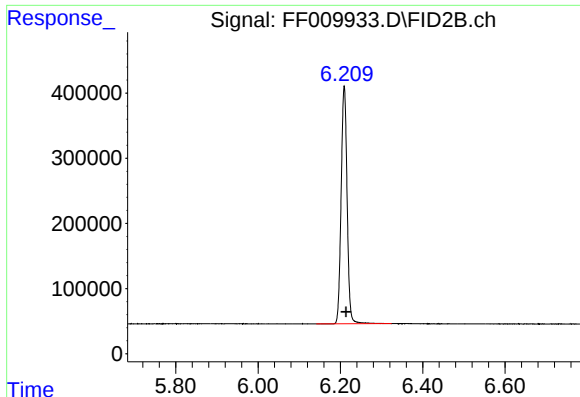

#3 N-DODECANE


R.T.: 6.209 min
Delta R.T.: -0.004 min
Response: 3651886
Conc: 26.57 ug/ml

Instrument :
FID_F
ClientSampleId :

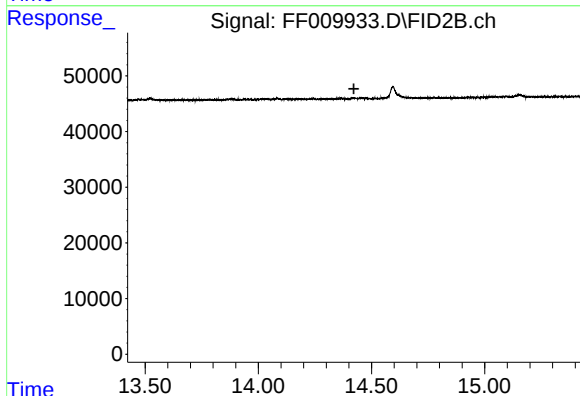


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

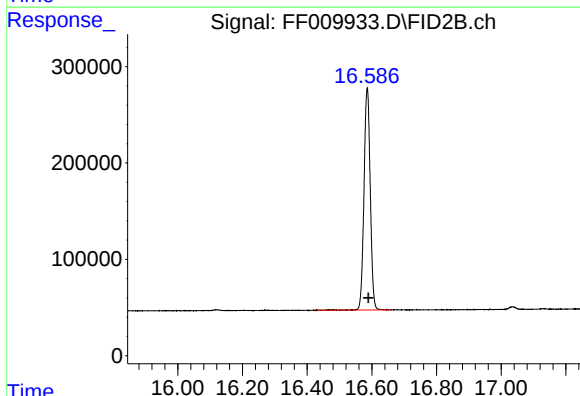


#12 N-OCTACOSANE

R.T.: 16.586 min
Delta R.T.: -0.004 min
Response: 3093469
Conc: 26.36 ug/ml

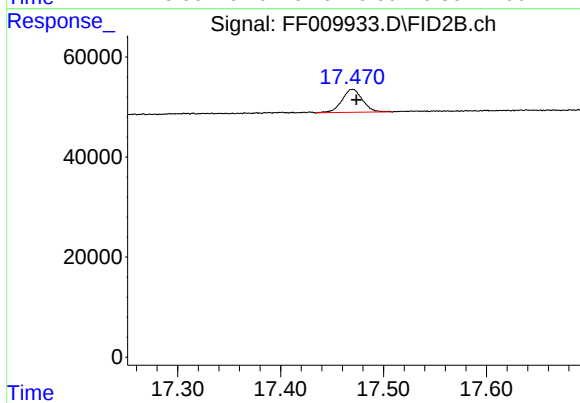

#13 N-TRIACONTANE


R.T.: 17.470 min
Delta R.T.: -0.004 min
Response: 63541
Conc: 0.55 ug/ml

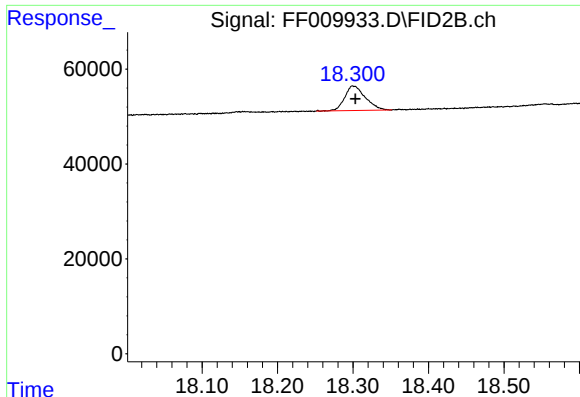

#14 N-DOTRIACONTANE


R.T.: 18.301 min
Delta R.T.: -0.002 min
Response: 97343
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

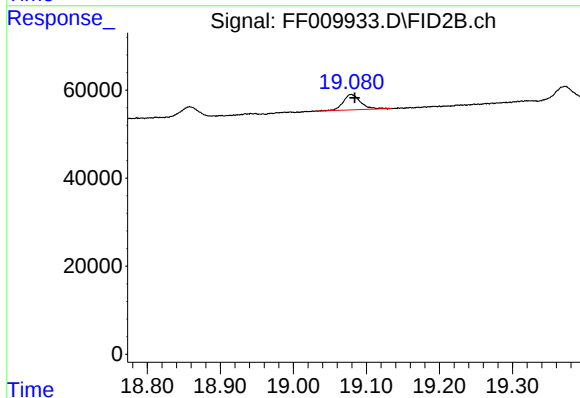

#15 N-TETRATRIACONTANE

R.T.: 19.079 min
Delta R.T.: -0.005 min
Response: 57940
Conc: 0.52 ug/ml

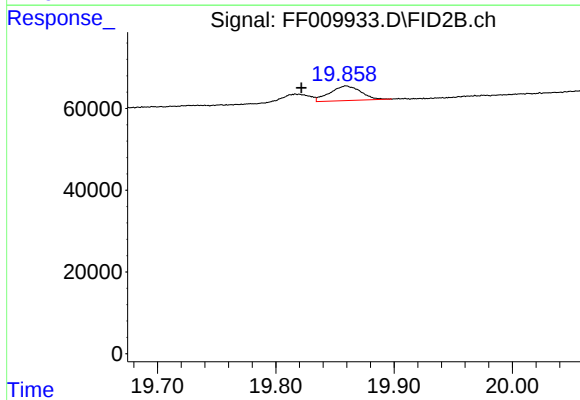

#16 N-HEXATRIACONTANE

R.T.: 19.860 min
Delta R.T.: 0.038 min
Response: 65082
Conc: 0.62 ug/ml