

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
 Data File : FF009934.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2022 14:09
 Operator : AJ\MA
 Sample : PB142653BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 15 00:42:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
 Quant Title :
 QLast Update : Fri Feb 11 12:58:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	3276279	30.312 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.590	171981	1.389 ug/ml
13) N-TRIACONTANE	17.467	47306	0.408 ug/ml
14) N-DOTRIACONTANE	18.306	103965	0.898 ug/ml
16) N-HEXATRIACONTANE	19.862	139410	1.324 ug/ml
18) N-TETRACONTANE	21.369	184321	1.984 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009934.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 14:09
Operator : AJ\MA
Sample : PB142653BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:42:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

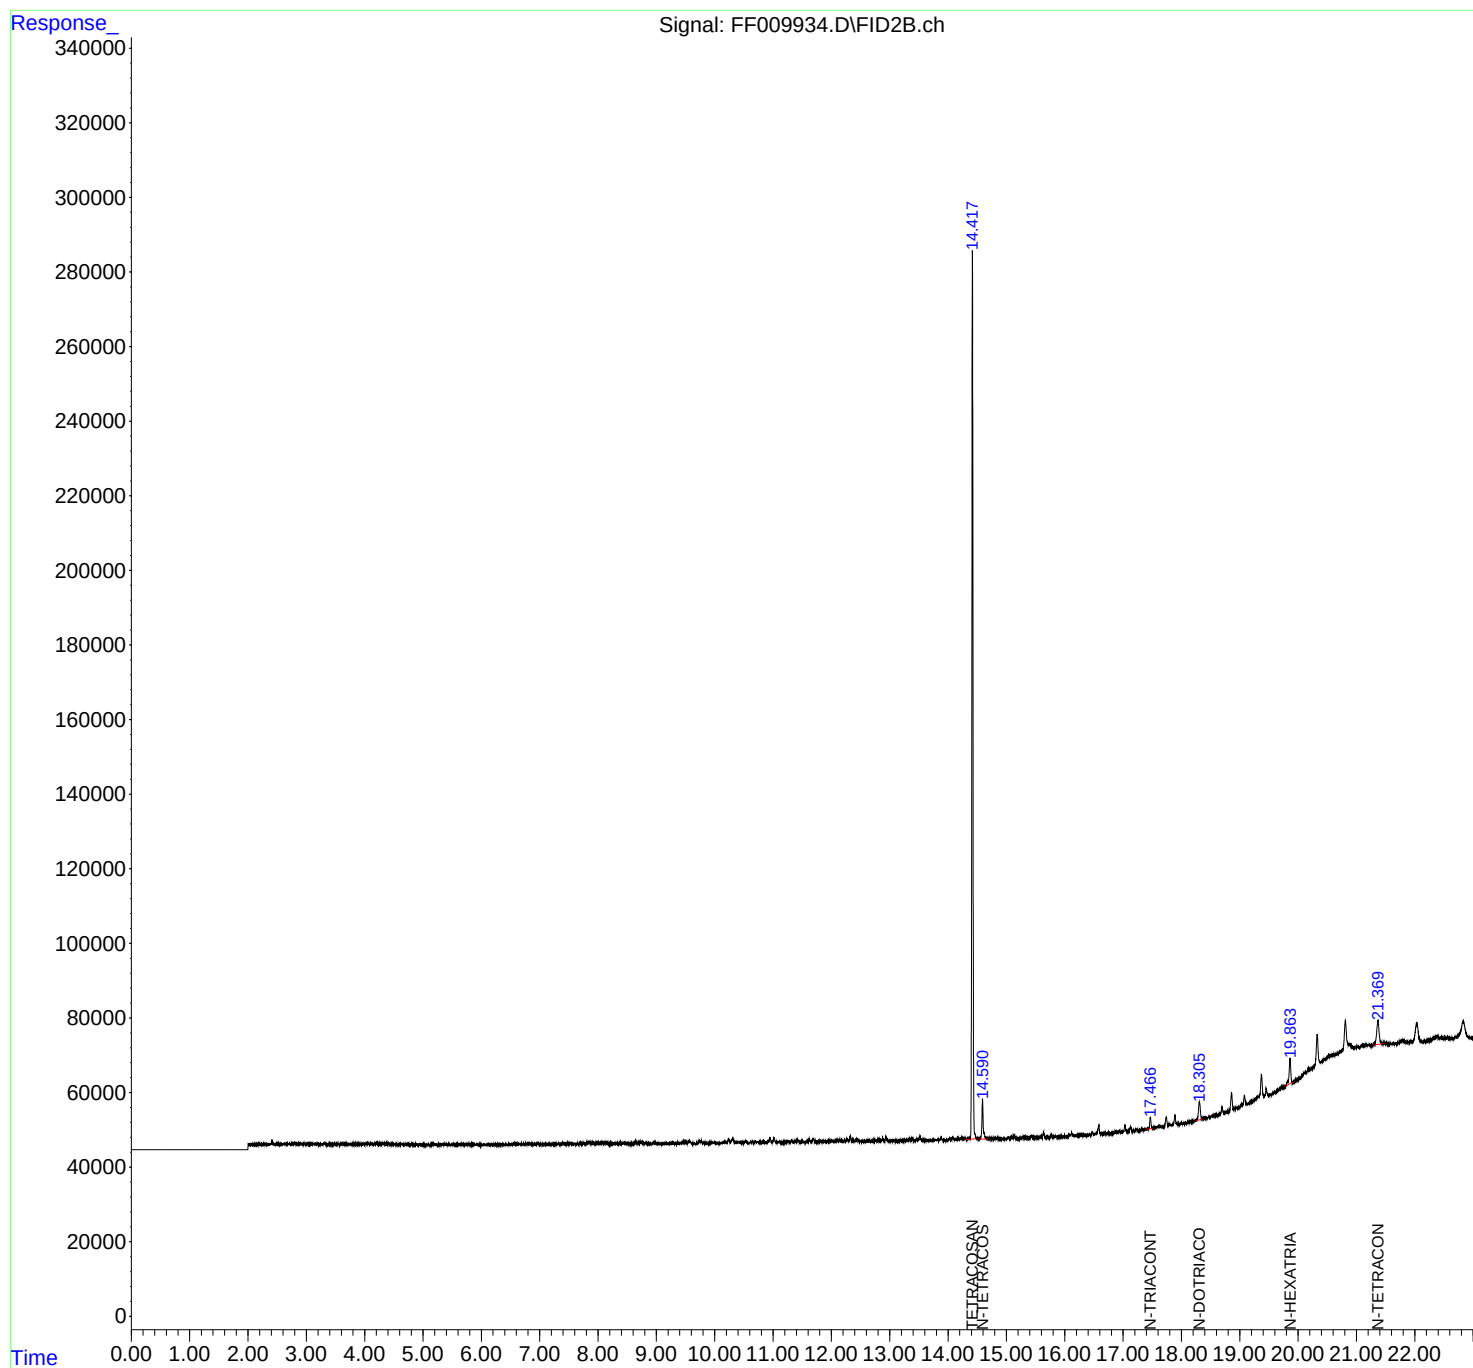

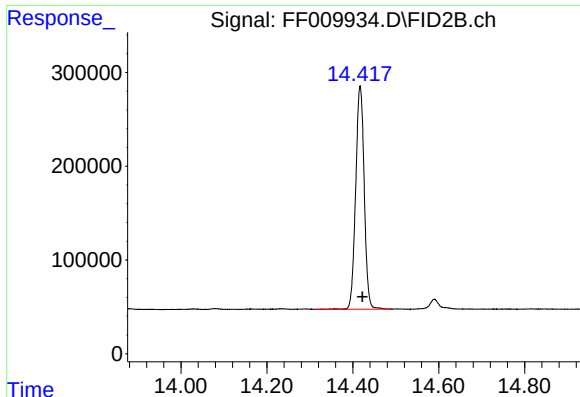


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.417 min
Delta R.T.: -0.005 min
Response: 3276279
Conc: 30.31 ug/ml

Instrument :


FID_F

ClientSampleId :

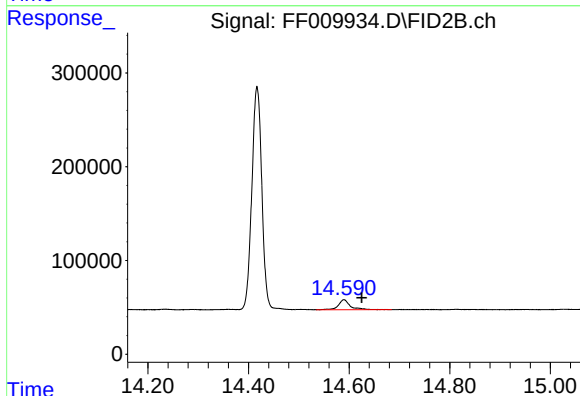


#10 N-TETRACOSANE

R.T.: 14.590 min
Delta R.T.: -0.035 min
Response: 171981
Conc: 1.39 ug/ml

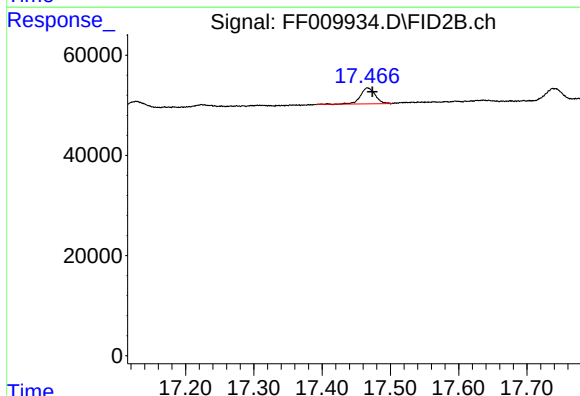


#13 N-TRIACONTANE

R.T.: 17.467 min
Delta R.T.: -0.007 min
Response: 47306
Conc: 0.41 ug/ml

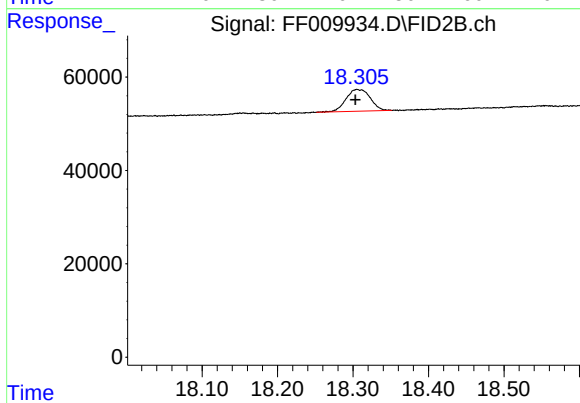

#14 N-DOTRIACONTANE


R.T.: 18.306 min
Delta R.T.: 0.003 min
Response: 103965
Conc: 0.90 ug/ml

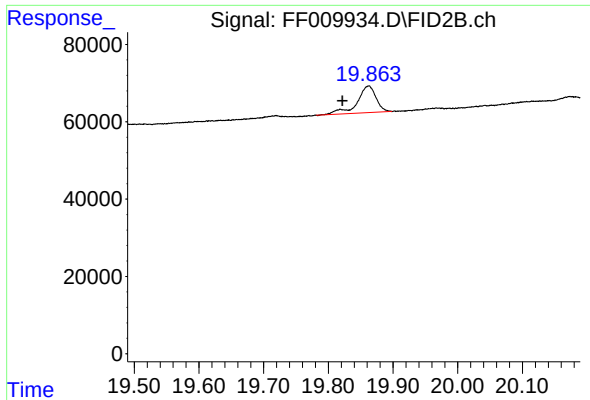

#16 N-HEXATRIACONTANE

R.T.: 19.862 min
Delta R.T.: 0.040 min
Response: 139410
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :

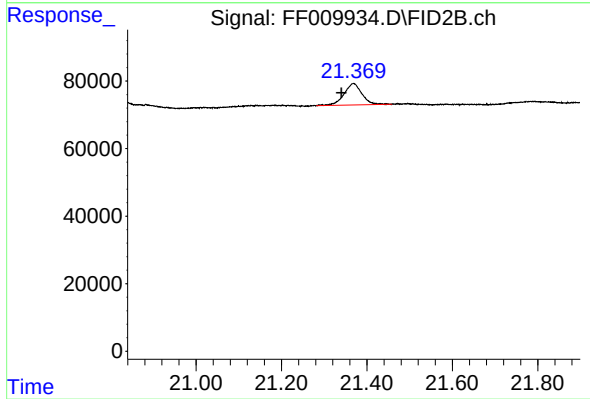

#18 N-TETRACONTANE

R.T.: 21.369 min
Delta R.T.: 0.028 min
Response: 184321
Conc: 1.98 ug/ml