

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009941.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 17:39
Operator : AJ\MA
Sample : N1527-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:44:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.418	2394761	22.157 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.469	43718	0.377 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009941.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 17:39
Operator : AJ\MA
Sample : N1527-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:44:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

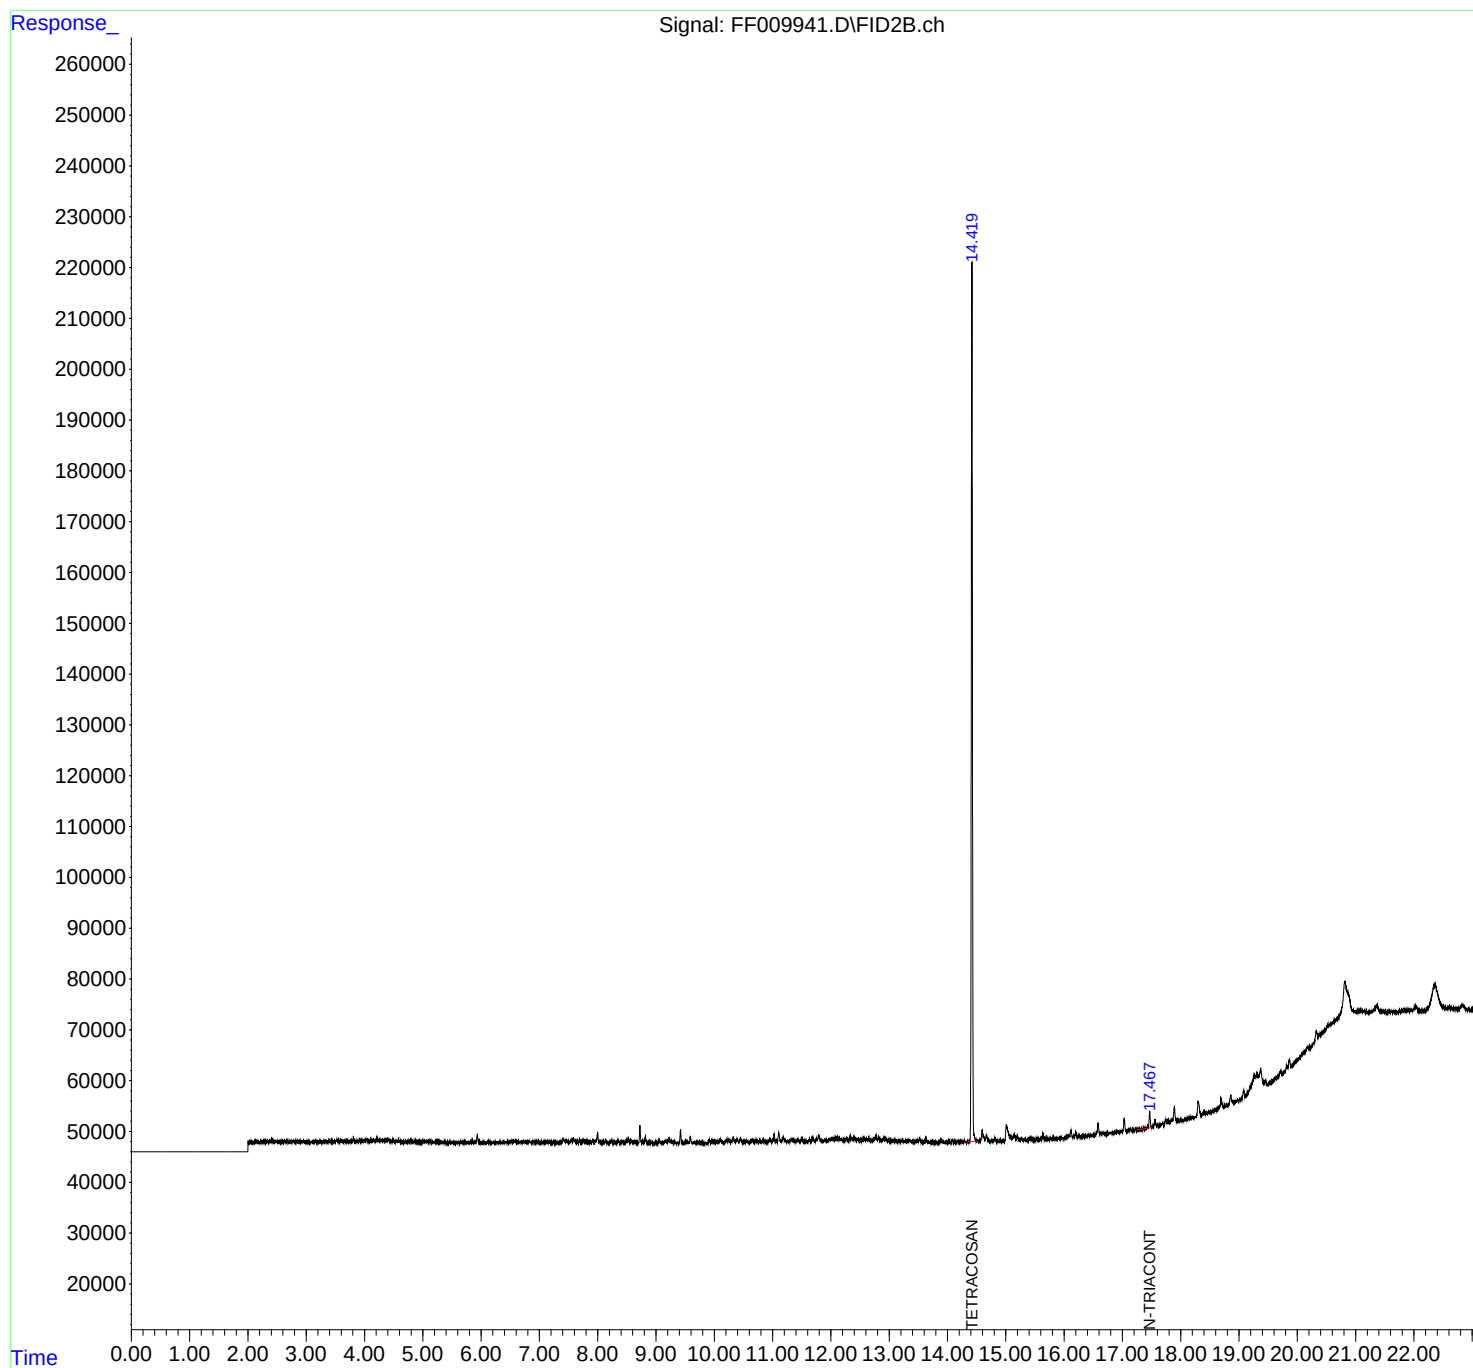


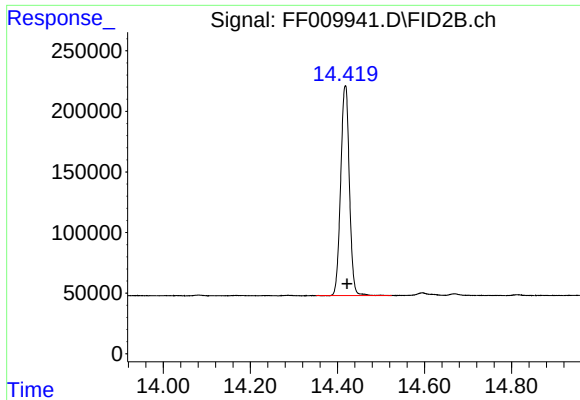

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.418 min
Delta R.T.: -0.004 min
Response: 2394761
Conc: 22.16 ug/ml

Instrument :
FID_F
ClientSampleId :

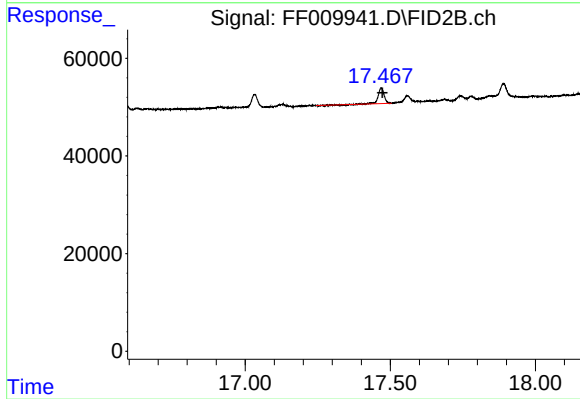

#13 N-TRIACONTANE

R.T.: 17.469 min
Delta R.T.: -0.005 min
Response: 43718
Conc: 0.38 ug/ml